


Mass Spectrum

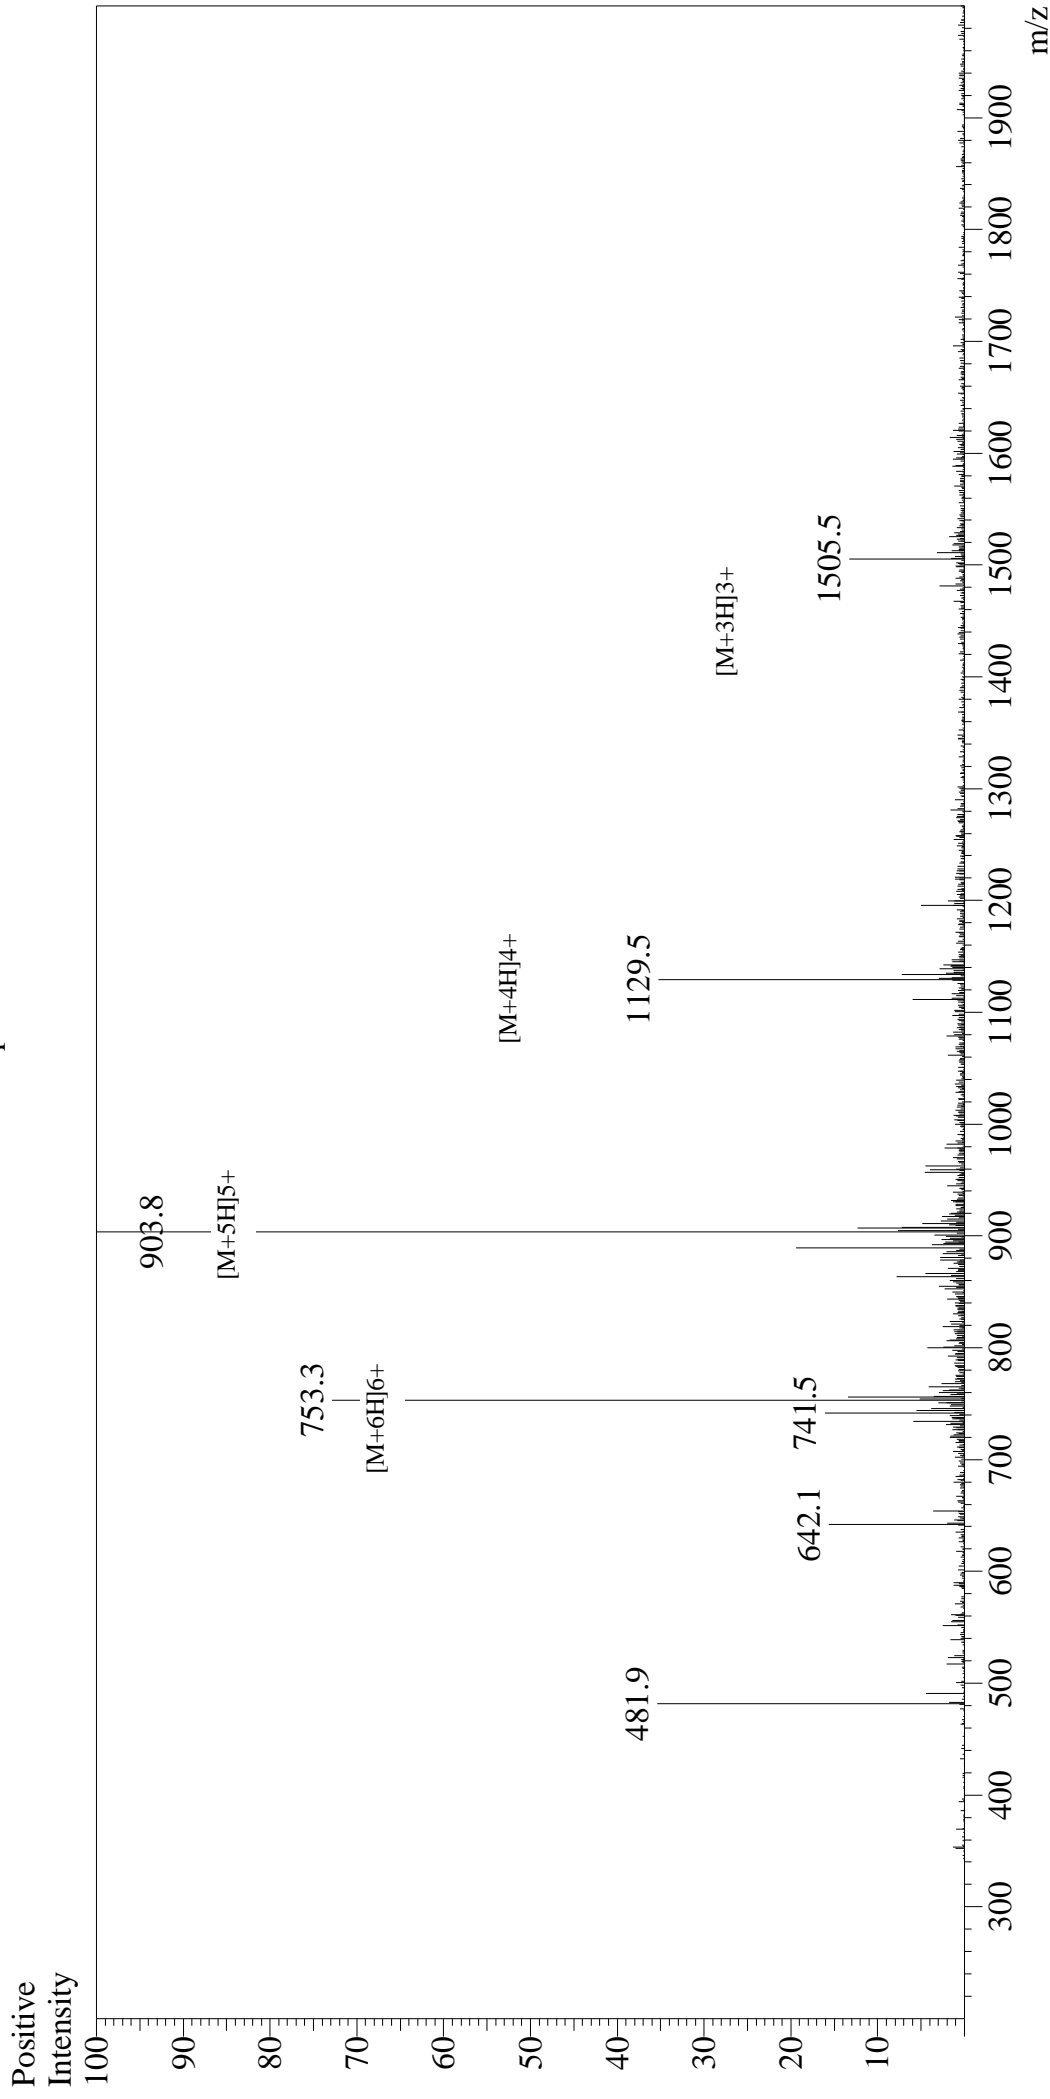

Sample Information

User : Gary
Month-Day Processed : 11/06/18
Time Processed : 15:02:31
Injection Volume : 1
Sample Name : β -Amyloid (1-42), human
Cat No. : RPI0017
Lot No. : PE5431809
Theoretical MW : 4514.10
Observed MW : 4514.0

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH