

Sample Name :CEF7, Influenza Virus NP (380-388)
 Cat No. :RP20419
 Lot No. :E2267320J
 Time Processed :6:21:48
 Month-Day-Year Processed :10/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

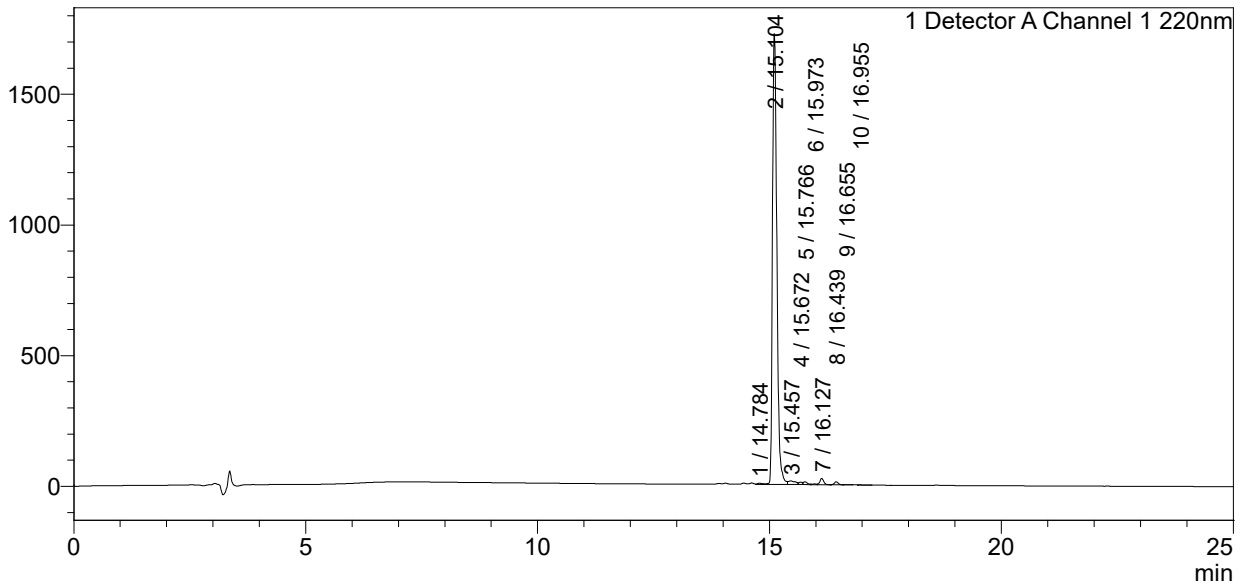

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.784	28280	4707	0.238
2	15.104	11371499	1724166	95.664
3	15.457	149287	14128	1.256
4	15.672	49250	9168	0.414
5	15.766	66037	10913	0.556
6	15.973	20409	2767	0.172
7	16.127	133263	24129	1.121
8	16.439	64663	11579	0.544
9	16.655	2100	280	0.018
10	16.955	2156	310	0.018
Total		11886943	1802147	100.000