

Sample Name : Dermorphin  
 Cat. No. : RP10427  
 Lot. No. : PE0701706

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

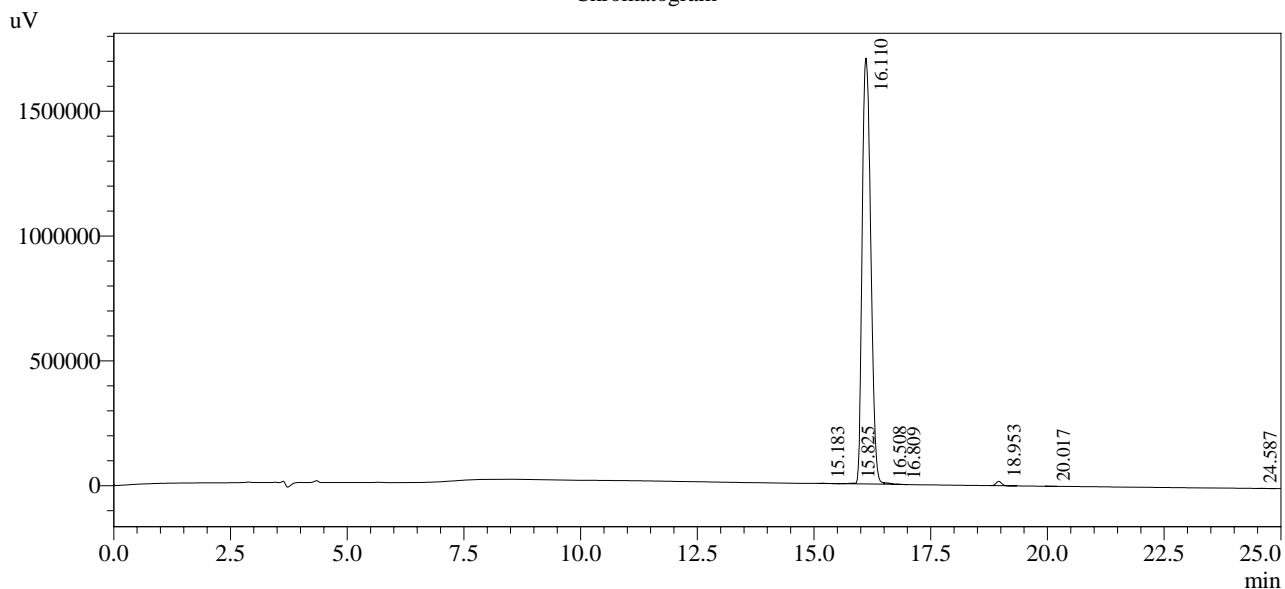

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.183	14365	1446	0.065
2	15.825	25760	2500	0.116
3	16.110	21887292	1706306	98.924
4	16.508	46544	5805	0.210
5	16.809	1808	224	0.008
6	18.953	145130	17619	0.656
7	20.017	1222	203	0.006
8	24.587	3314	358	0.015
Total		22125435	1734460	100.000