

Sample Name : Fibronectin CS1 Peptide
 Cat. No. : RP 10838
 Lot. No. : PE1831610

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

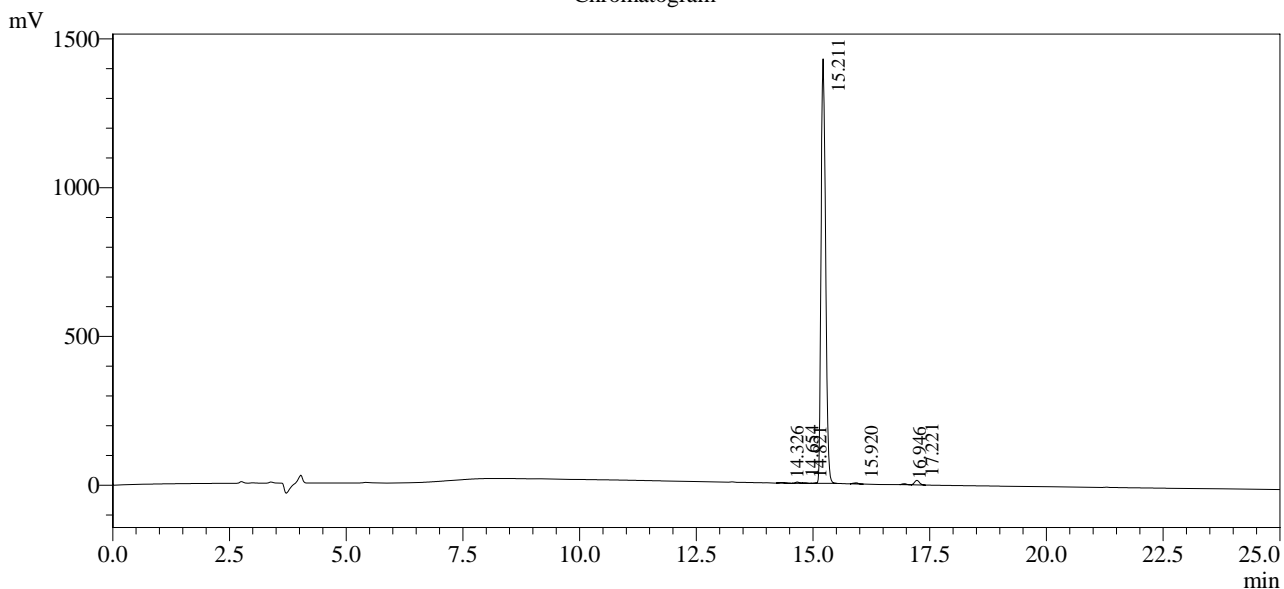

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.326	15604	1941	0.157
2	14.654	28016	4004	0.283
3	14.821	9069	1517	0.092
4	15.211	9698817	1426453	97.877
5	15.920	27393	3686	0.276
6	16.946	20408	3488	0.206
7	17.221	109932	15238	1.109
Total		9909238	1456326	100.000