


Mass Spectrum

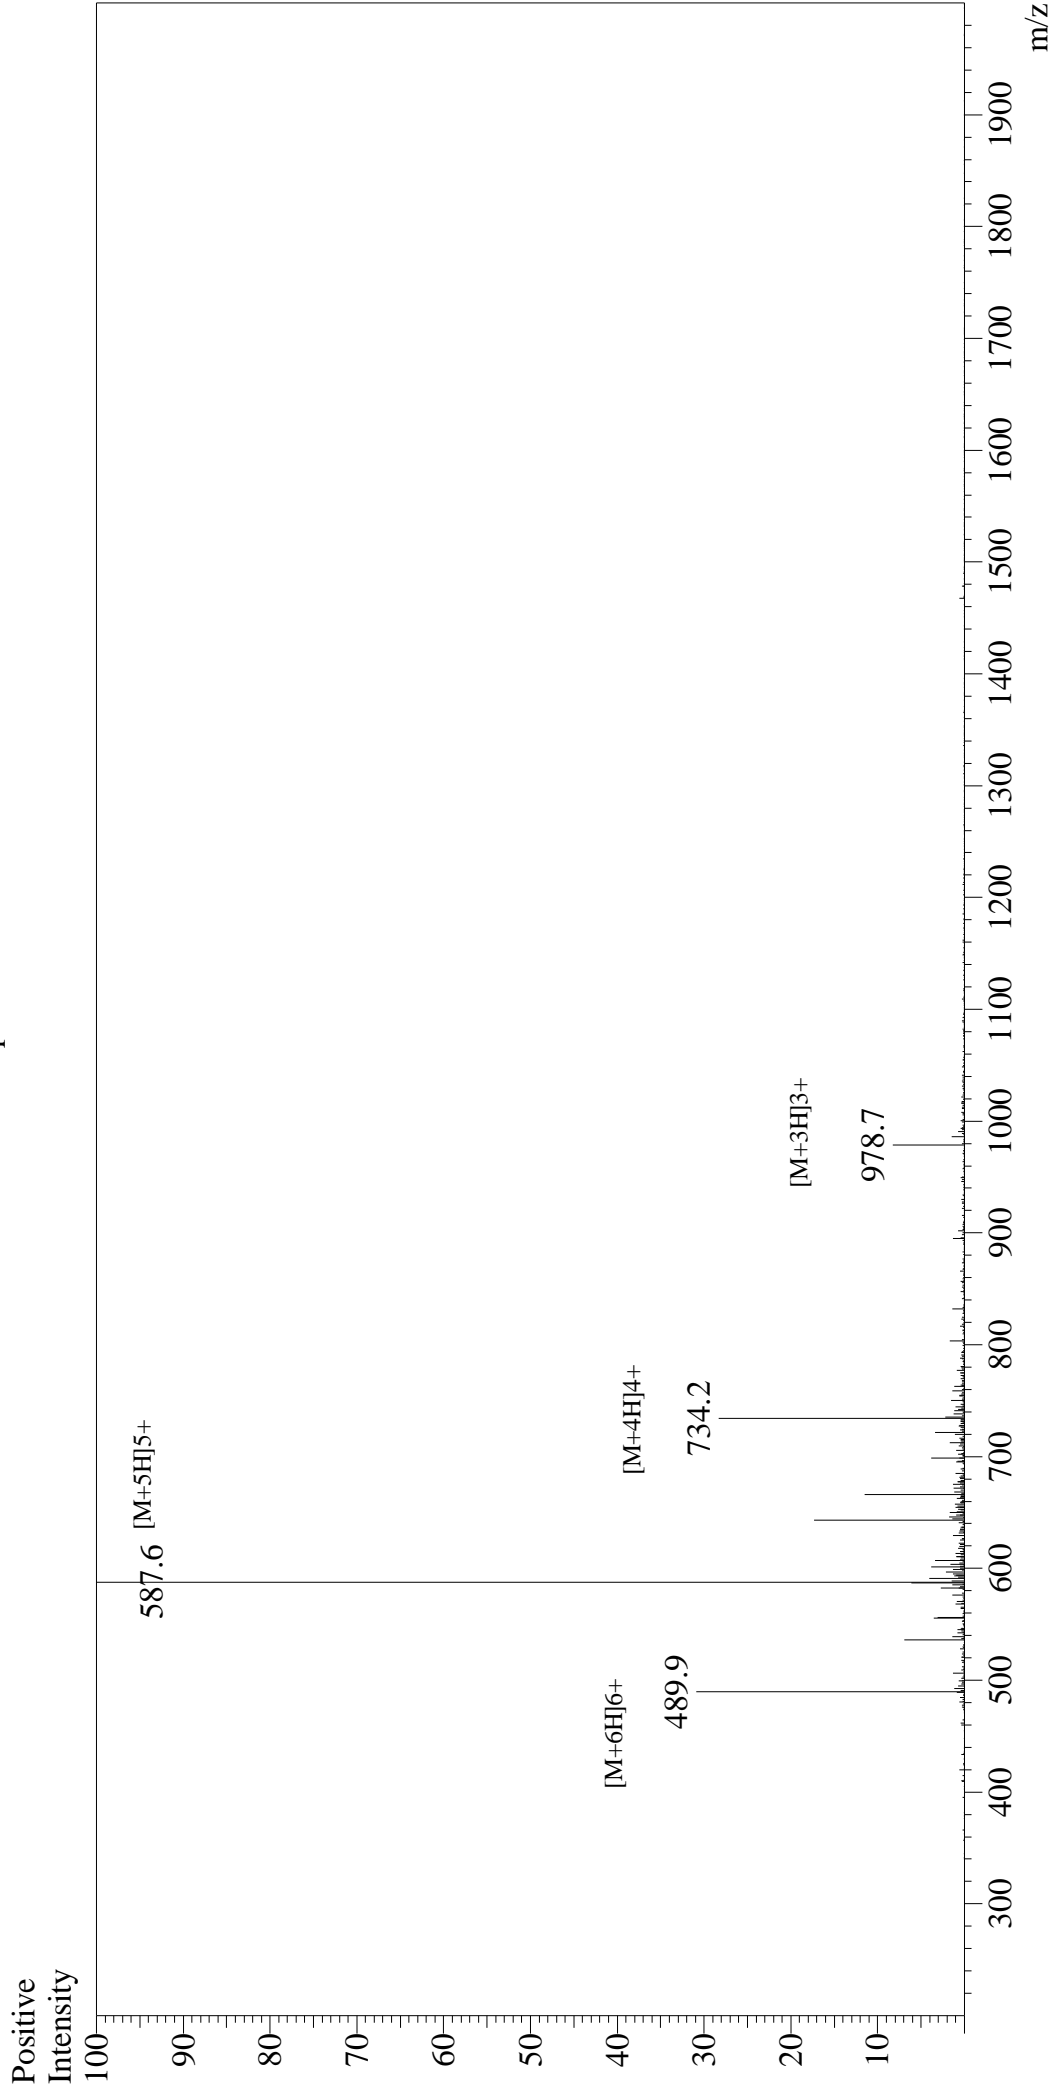

Sample Information

User : Gary
Month-Day Processed : 11/02/18
Time Processed : 20:19:18
Injection Volume : 0.2
Sample Name : ACTH (1-24), human
Cat No. : RP11303
Lot No. : PE0261811
Theoretical MW : 2933.44
Observed MW : 2933.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH