


Mass Spectrum

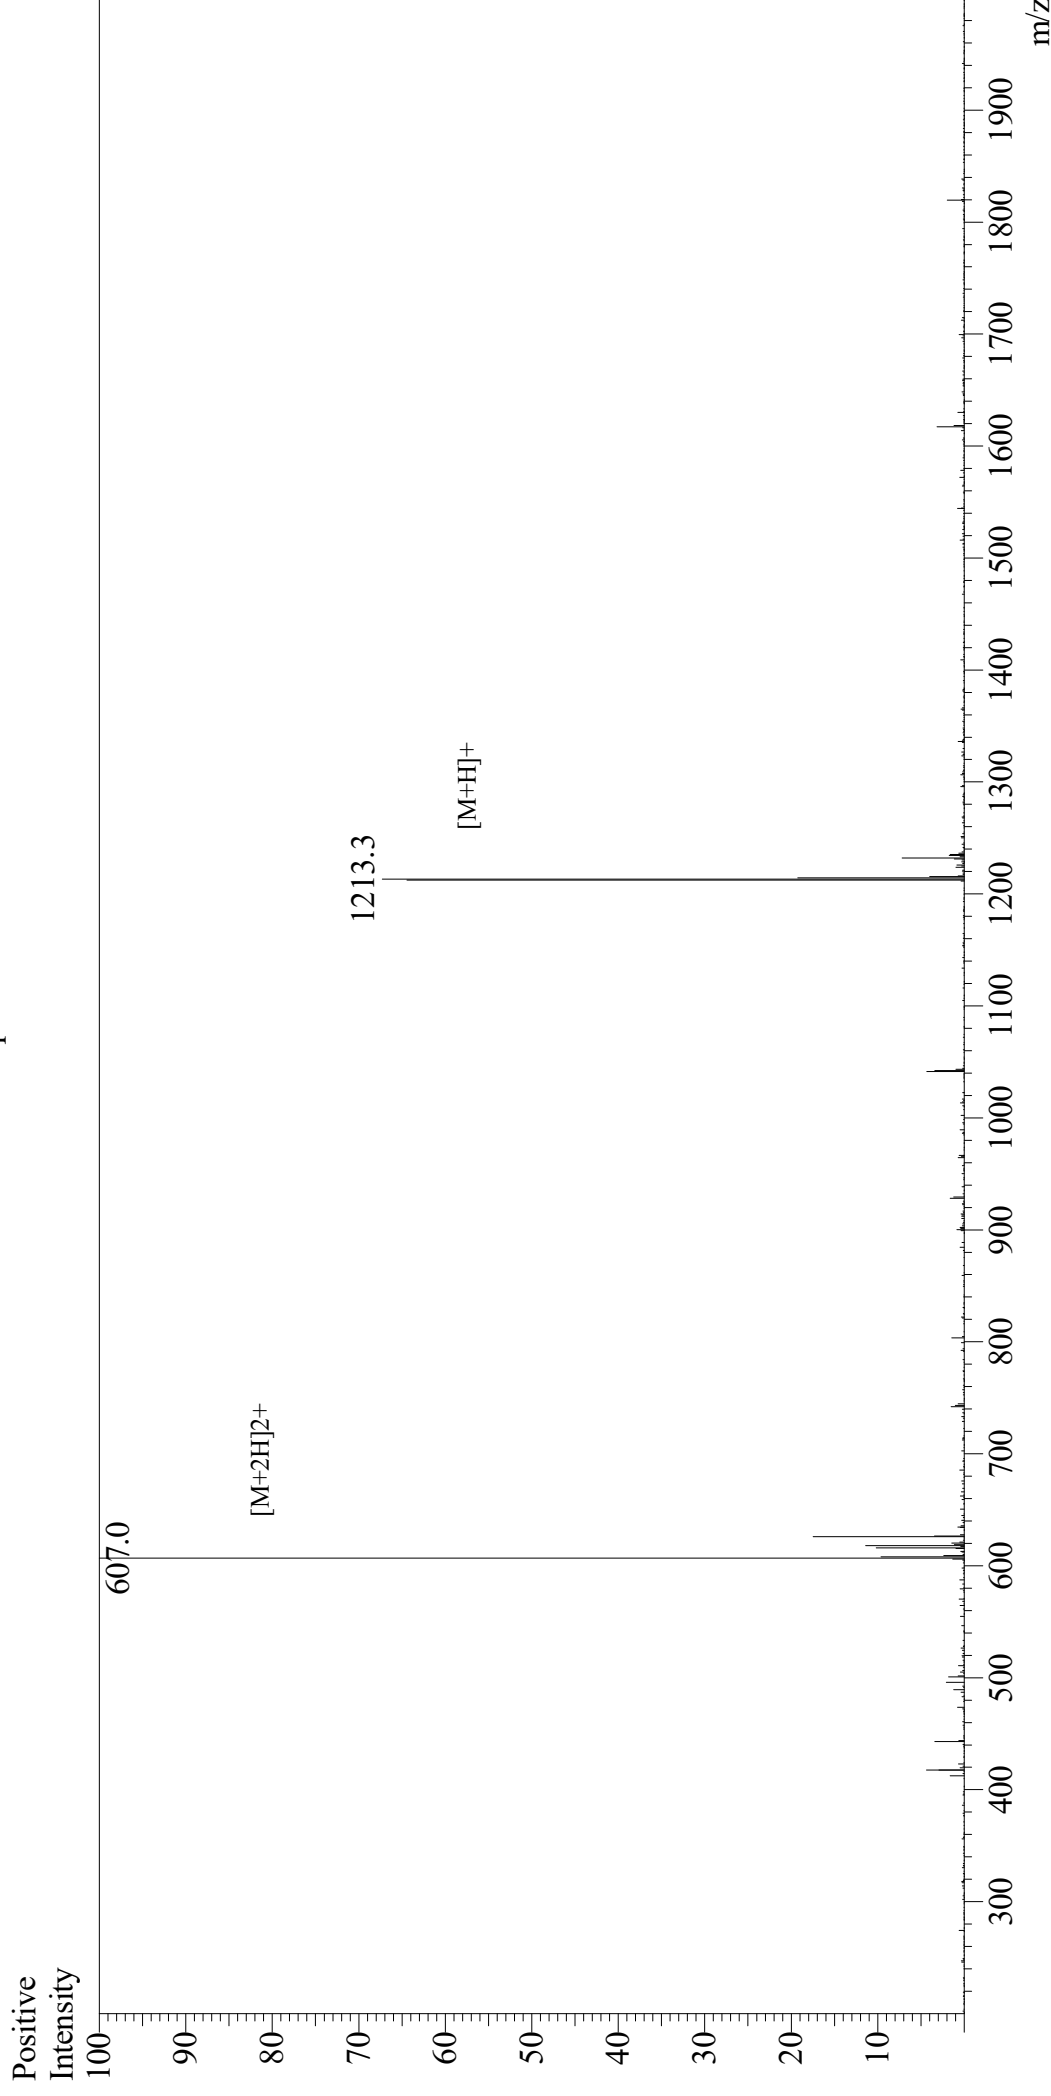

Sample Information

User : Gary
Month-Day Processed : 06/24/20
Time Processed : 01:28:55 PM
Injection Volume : 0.3
Sample Name : Luteinizing Hormone Releasing Hormone (LH-RH), salmon
Cat No. : RP10673
Lot No. : E5395820F
Theoretical MW : 1212.31
Observed MW : 1212.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH