

Sample Name :Ghrelin, rat
 Cat No. :RP10781
 Lot No. :E7122820L
 Time Processed : 11:29:06
 Month-Day-Year Processed : 12/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

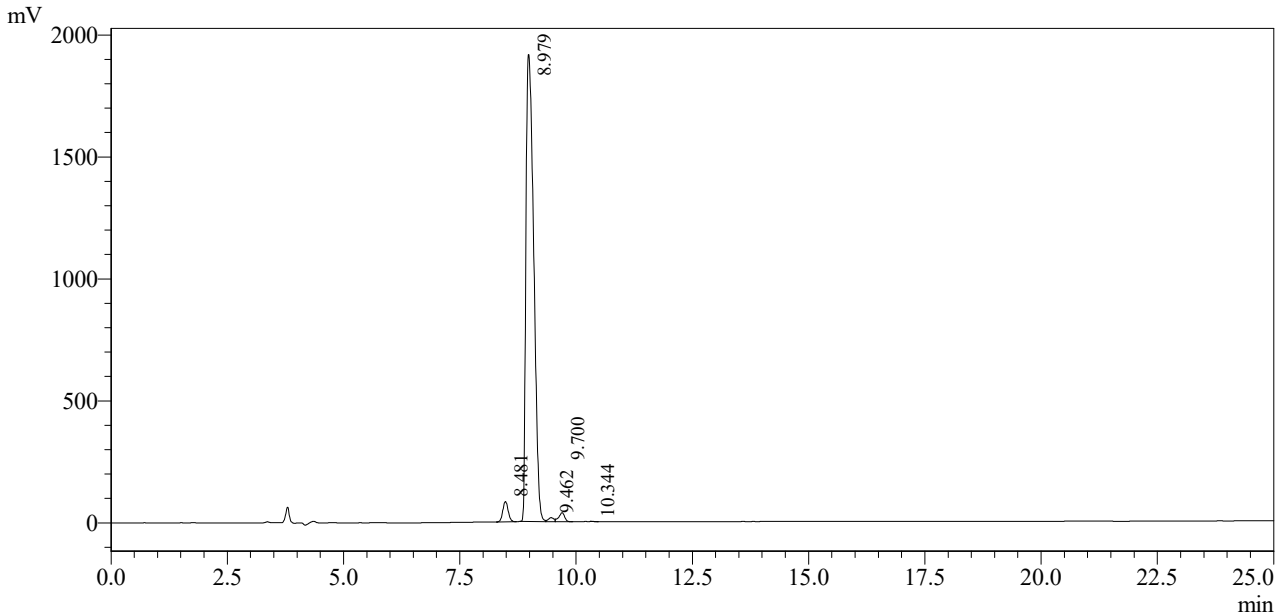

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.481	669113	83761	2.864
2	8.979	22241024	1913749	95.186
3	9.462	135998	16205	0.582
4	9.700	317448	37144	1.359
5	10.344	2309	658	0.010
Total		23365891	2051517	100.000