

Sample Name :Colivelin
 Cat No. :RP20167
 Lot No. :E4026820H
 Time Processed : 6:41:44
 Month-Day-Year Processed : 09/05/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|--------------|-------|
| 0.01 | Pumps | Pump B Conc. | 5 |
| 25.00 | Pumps | Pump B Conc. | 65 |
| 25.01 | Pumps | Pump B Conc. | 95 |
| 27.00 | Pumps | Pump B Conc. | 95 |
| 27.01 | Pumps | Pump B Conc. | 5 |
| 32.00 | Pumps | Pump B Conc. | 5 |
| 32.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

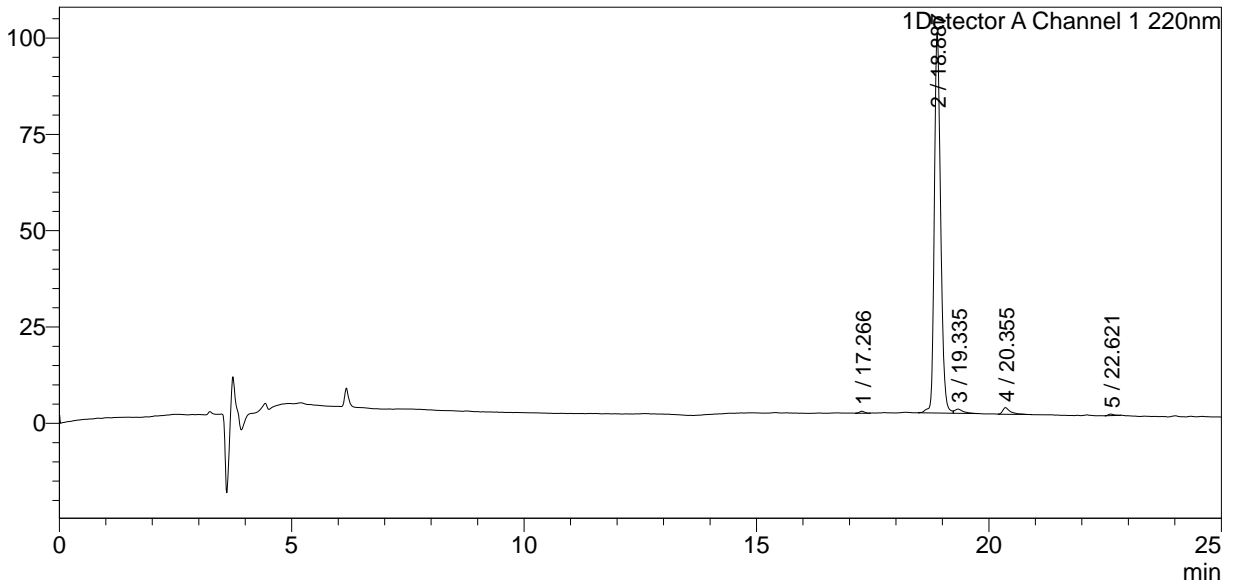

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|--------|--------|---------|
| 1 | 17.266 | 3733 | 503 | 0.385 |
| 2 | 18.887 | 929844 | 97824 | 95.863 |
| 3 | 19.335 | 13355 | 1081 | 1.377 |
| 4 | 20.355 | 19789 | 1695 | 2.040 |
| 5 | 22.621 | 3248 | 380 | 0.335 |
| Total | | 969970 | 101483 | 100.000 |