

Sample Name :Myelin Basic Protein (MBP) (68-82), guinea pig
 Cat No. :RP10605
 Lot No. :E4775219J
 Time Processed :8:01:39 AM
 Month-Day-Year Processed :10/24/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

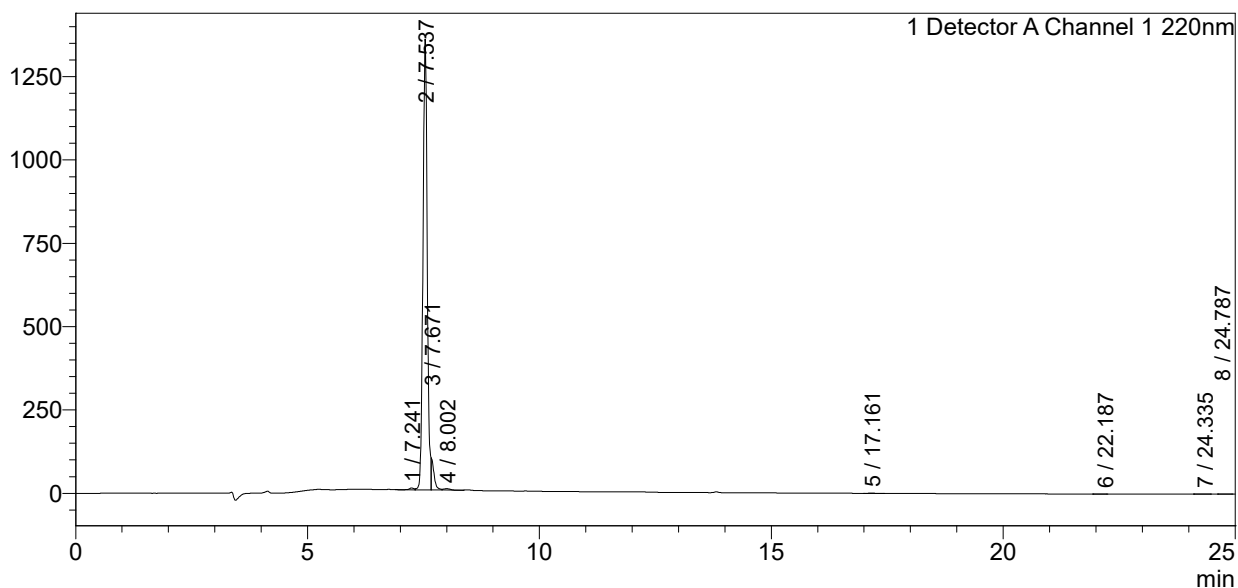

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.241	35190	5436	0.384
2	7.537	8713323	1352818	95.007
3	7.671	378583	96421	4.128
4	8.002	34948	4167	0.381
5	17.161	3219	257	0.035
6	22.187	1203	117	0.013
7	24.335	1029	77	0.011
8	24.787	3715	454	0.041
Total		9171210	1459747	100.000