

Sample Name :Fibrinogen Binding Inhibitor Peptide
Cat No. :RP10832
Lot No. :E4780519I
Time Processed :10:17:55
Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment:ZJ17010507

<Chromatogram>

mV

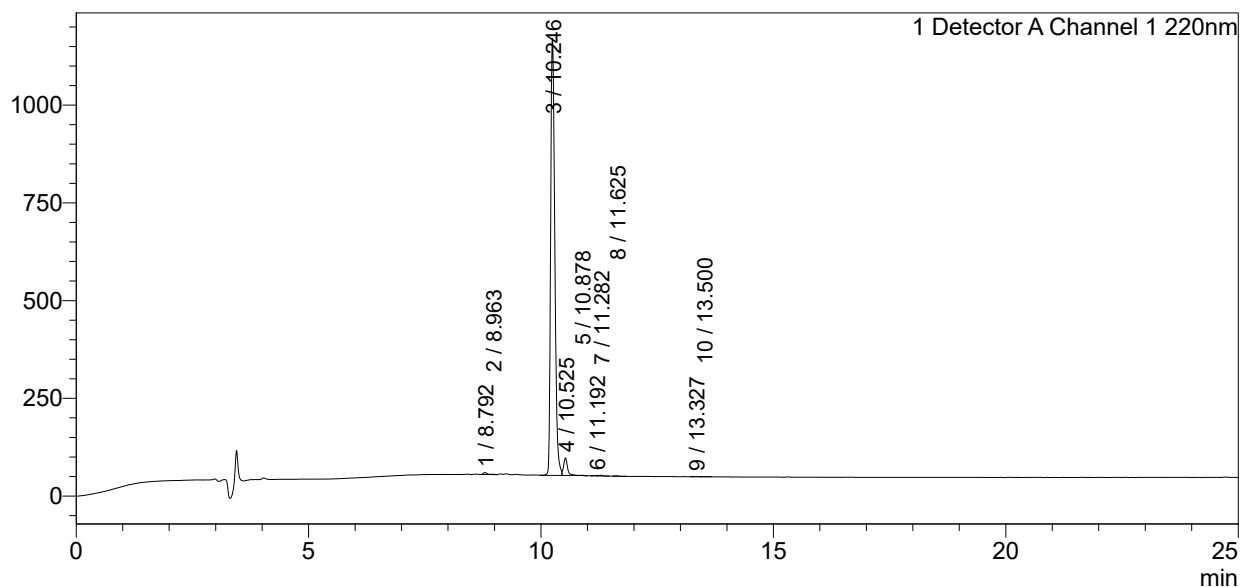

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.792	27218	5062	0.375
2	8.963	4032	941	0.056
3	10.246	6940896	1117149	95.576
4	10.525	258763	44960	3.563
5	10.878	3587	780	0.049
6	11.192	4674	892	0.064
7	11.282	10694	1982	0.147
8	11.625	6897	1134	0.095
9	13.327	3305	437	0.046
10	13.500	2106	270	0.029
Total		7262171	1173607	100.000