


Mass Spectrum

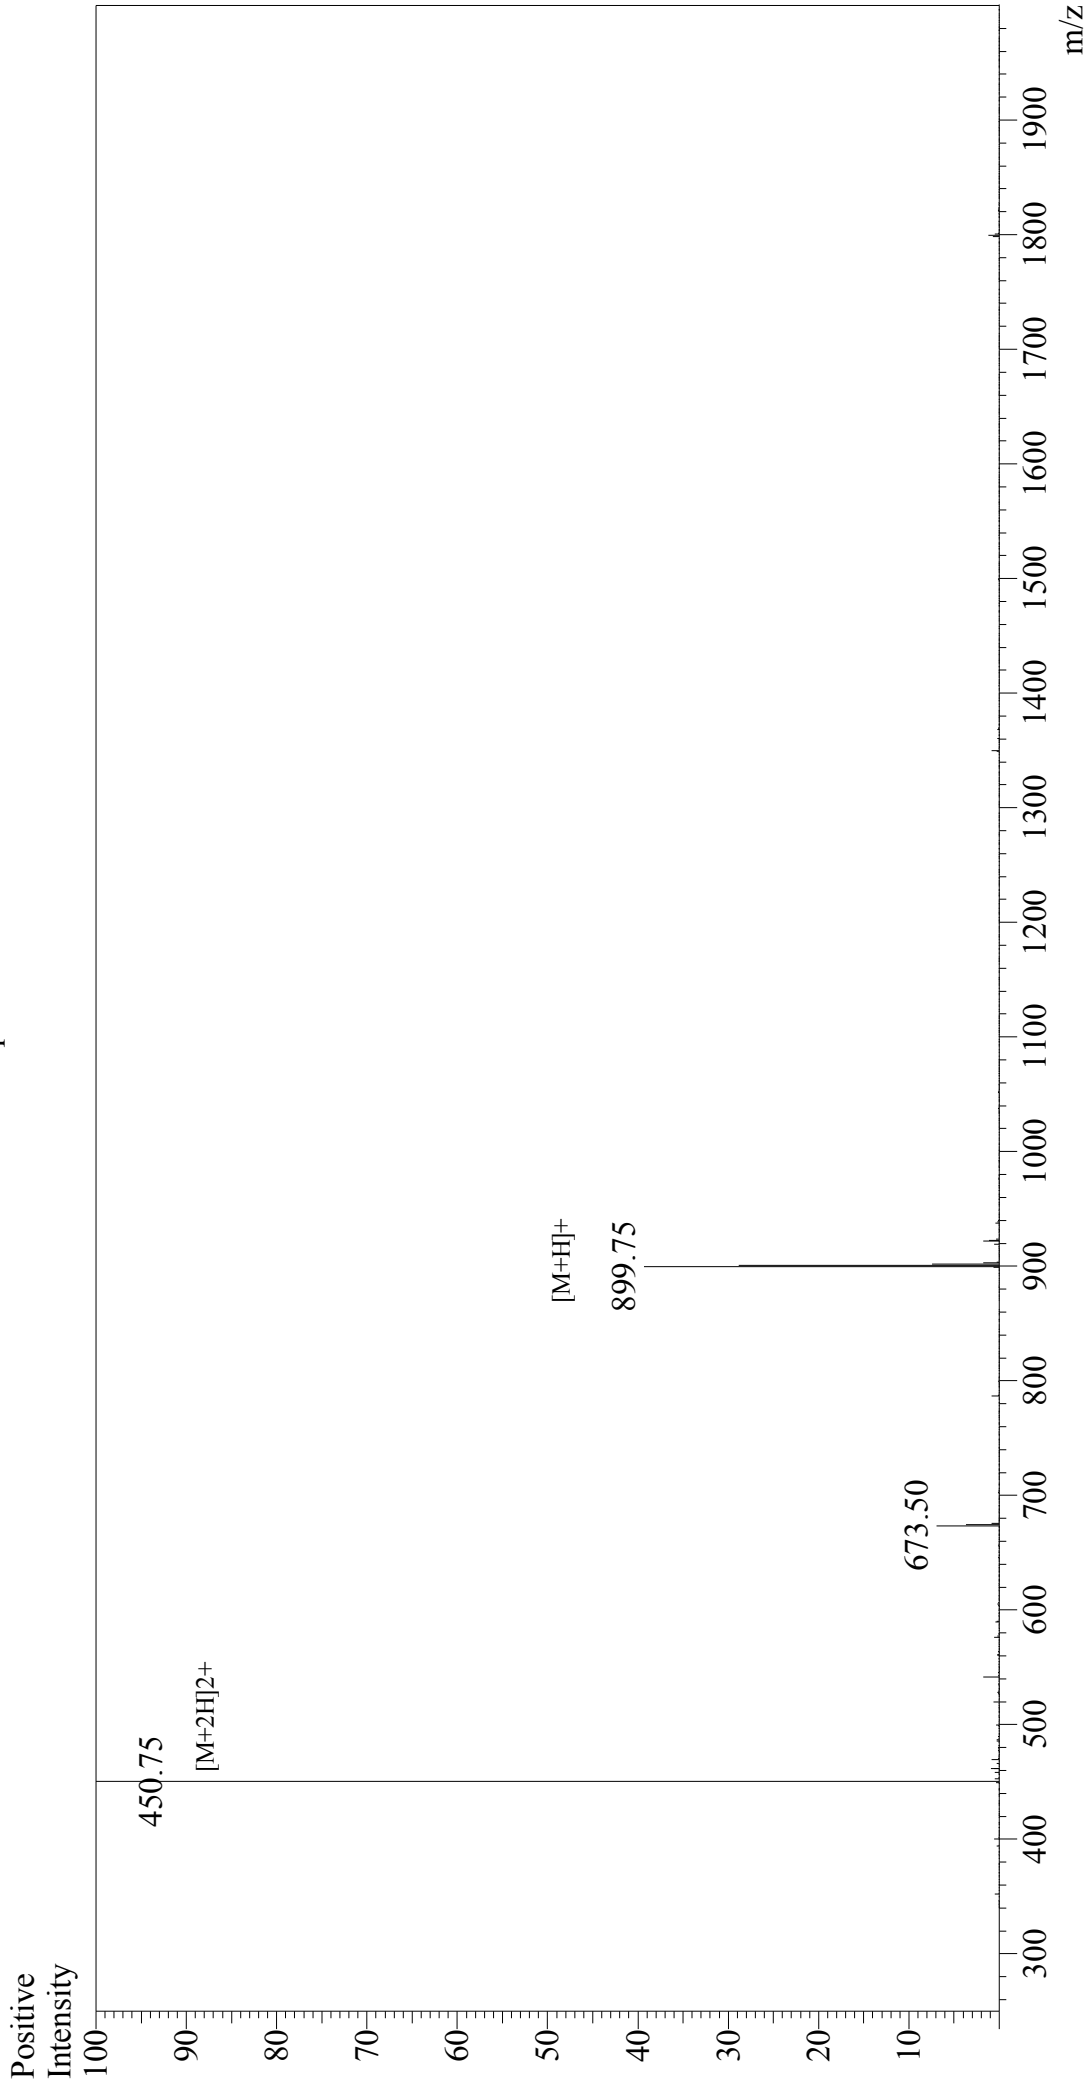

Sample Information

Acquired by : Gary
Month-Day Processed : 12/27/17
Time Processed : 17:06:56
Injection Volume : 0.2

Sample Name : Cardiotoxin Analog (CTX) IV (6-12)
Cat. No. : RP17303
Lot. No. : PE2721712
Theoretical MW : 899.14
Observed MW : 899.50

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH