

Sample Name: N-Acetyl-Ser-Asp-Lys-Pro
 Cat No.: RP10555
 Lot No.: E5289120A
 Time Processed :8:07:12
 Month-Day-Year Processed :01/10/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

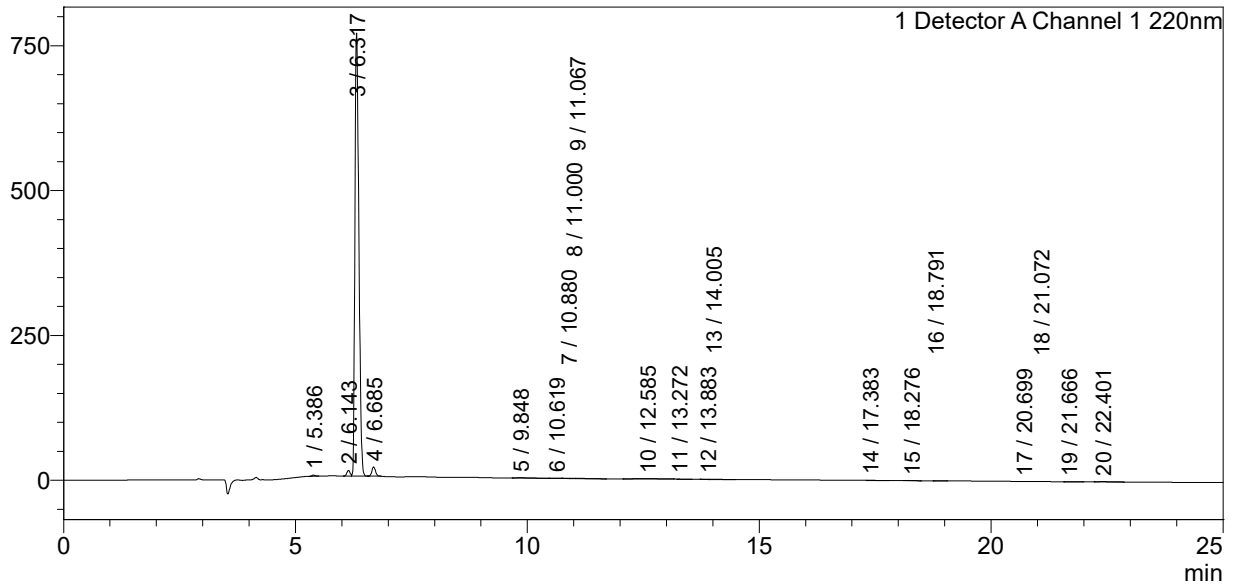

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.386	8993	1742	0.189
2	6.143	47222	9919	0.992
3	6.317	4531088	764953	95.179
4	6.685	87707	16126	1.842
5	9.848	14218	896	0.299
6	10.619	1089	103	0.023
7	10.880	1086	190	0.023
8	11.000	1937	311	0.041
9	11.067	9484	351	0.199
10	12.585	26032	836	0.547
11	13.272	1272	77	0.027
12	13.883	1355	194	0.028
13	14.005	6002	343	0.126
14	17.383	3080	187	0.065
15	18.276	2400	204	0.050

Peak#	Ret. Time	Area	Height	Area%
16	18.791	1632	136	0.034
17	20.699	3218	303	0.068
18	21.072	1069	130	0.022
19	21.666	2163	157	0.045
20	22.401	9557	931	0.201
Total		4760604	798089	100.000