


Mass Spectrum

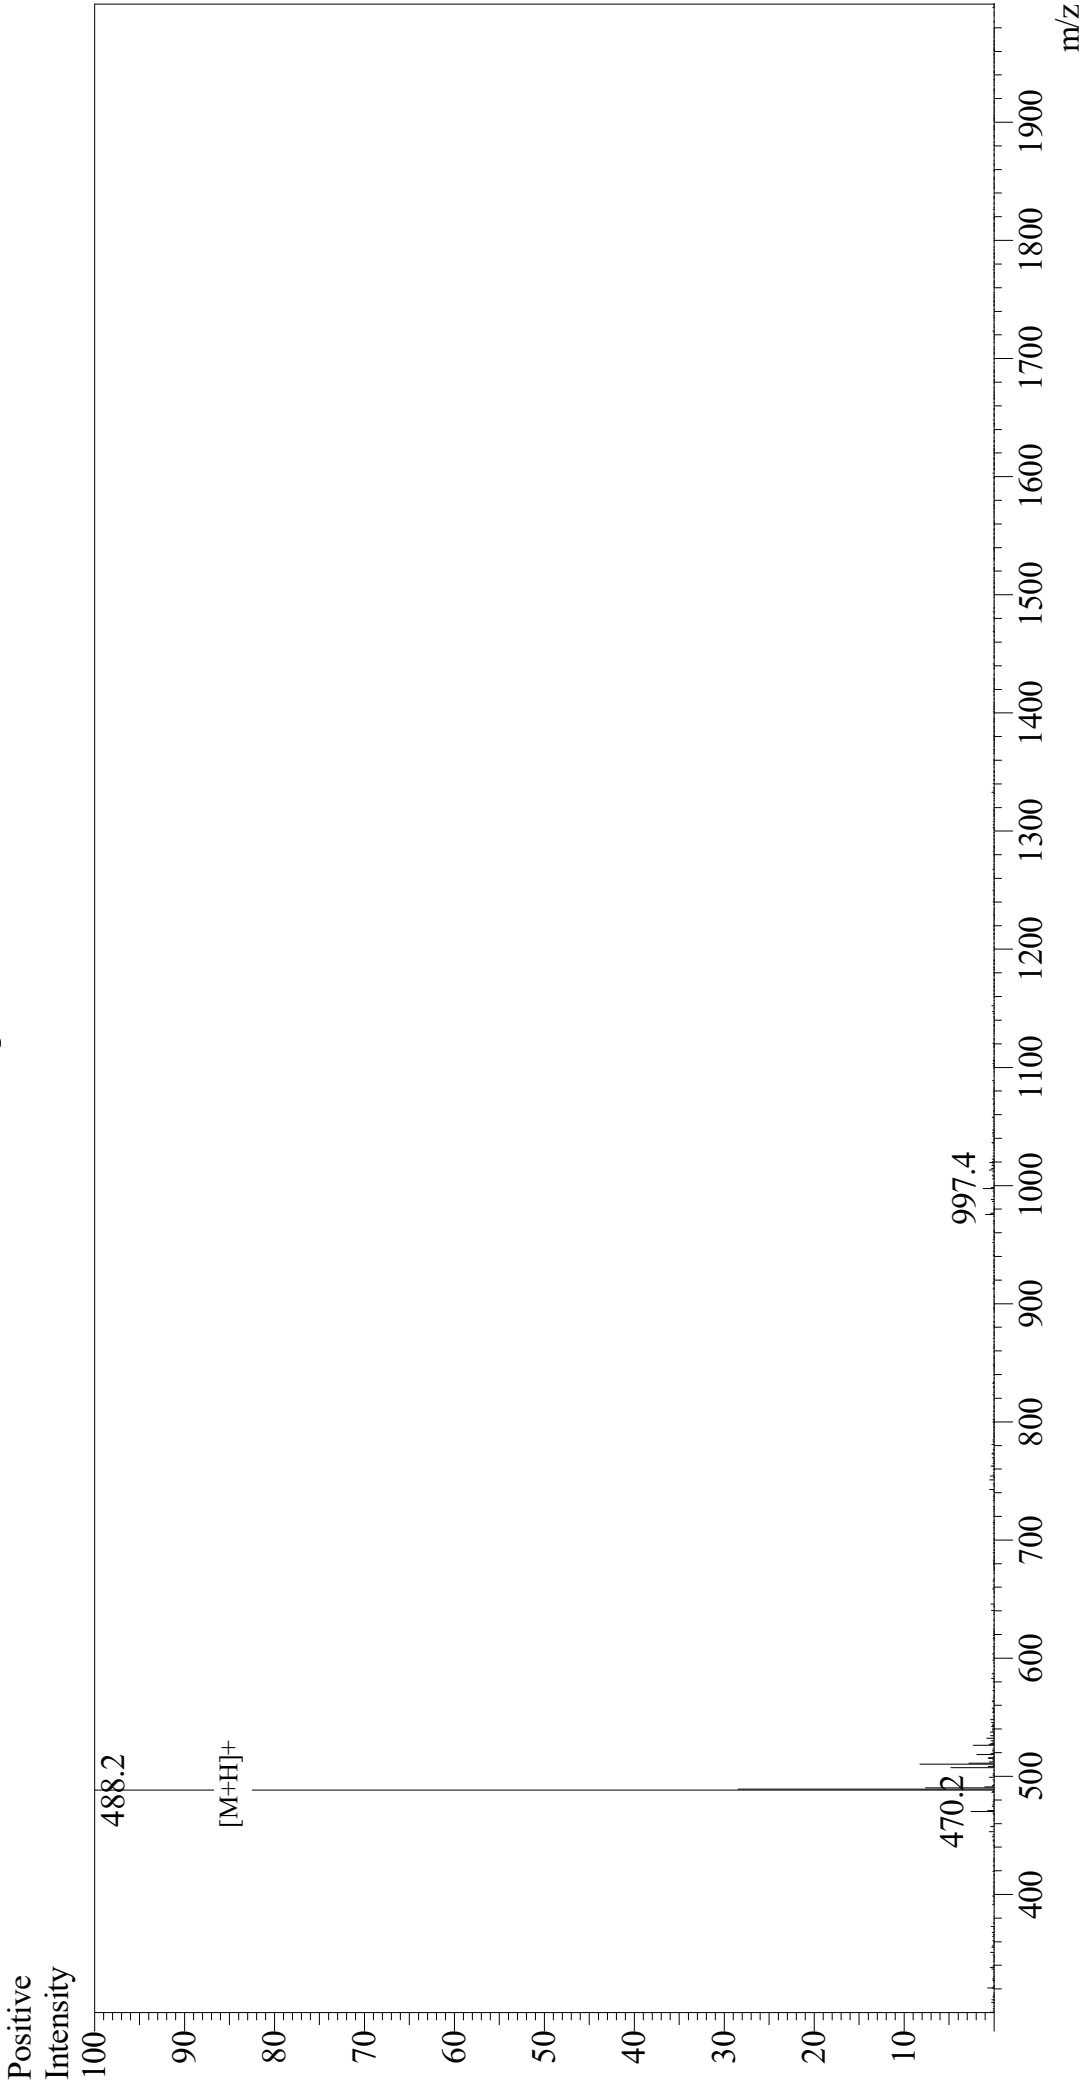

Sample Information

Acquired by: Gary
Month-Day Processed: 01/09/20
Time Processed: 04:32:50 PM
Injection Volume: 0.3
Sample Name: N-Acetyl-Ser-Asp-Lys-Pro
Cat No.: RPI0555
Lot No.: E5289120A
Theoretical MW: 487.50
Observed MW: 487.2

Interface: ESI
Nebulizing Gas Flow: 1.5L/min
CDL Temp: 250
Block Temp: 200

Equipment: GK11010007
Interface Bias: +4.5 kV
Drying Gas Flow: 5 L/min
T.Flow: 0.2 ml/min
B.conc: 50% H₂O/50% MeOH