

Sample Name :BMf-BH3
 Cat No. :RP20201
 Lot No. :E4855019I
 Time Processed :5:48:05 AM
 Month-Day-Year Processed :09/26/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

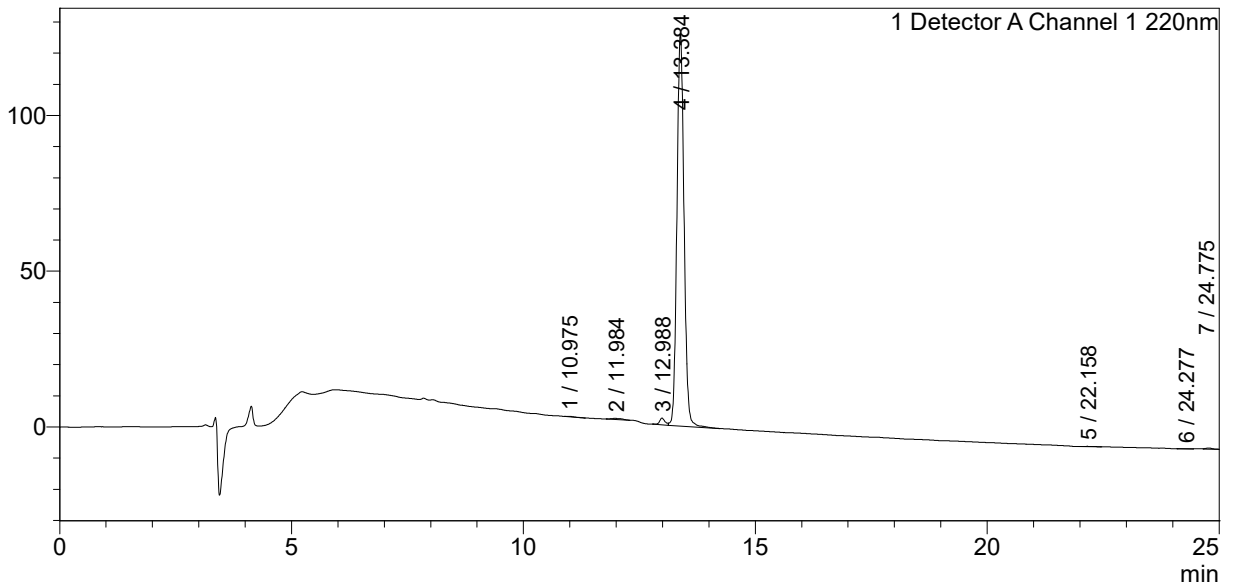

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.975	1359	133	0.099
2	11.984	5465	322	0.399
3	12.988	17622	2159	1.288
4	13.384	1337306	125810	97.741
5	22.158	1693	109	0.124
6	24.277	1405	85	0.103
7	24.775	3359	351	0.246
Total		1368210	128969	100.000