

Sample Name :Angiotensin II, human
Cat. No. : RP11257
Lot. No. : E6894121F
Time Processed :12:11:15 PM
Month-Dav-Year Processed :06/04/2021
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	0
5.00	Pumps	Pump A B.Conc	0
20.00	Pumps	Pump A B.Conc	30
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	0
35.00	Pumps	Pump A B.Conc	0
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

<Chromatogram>

mV

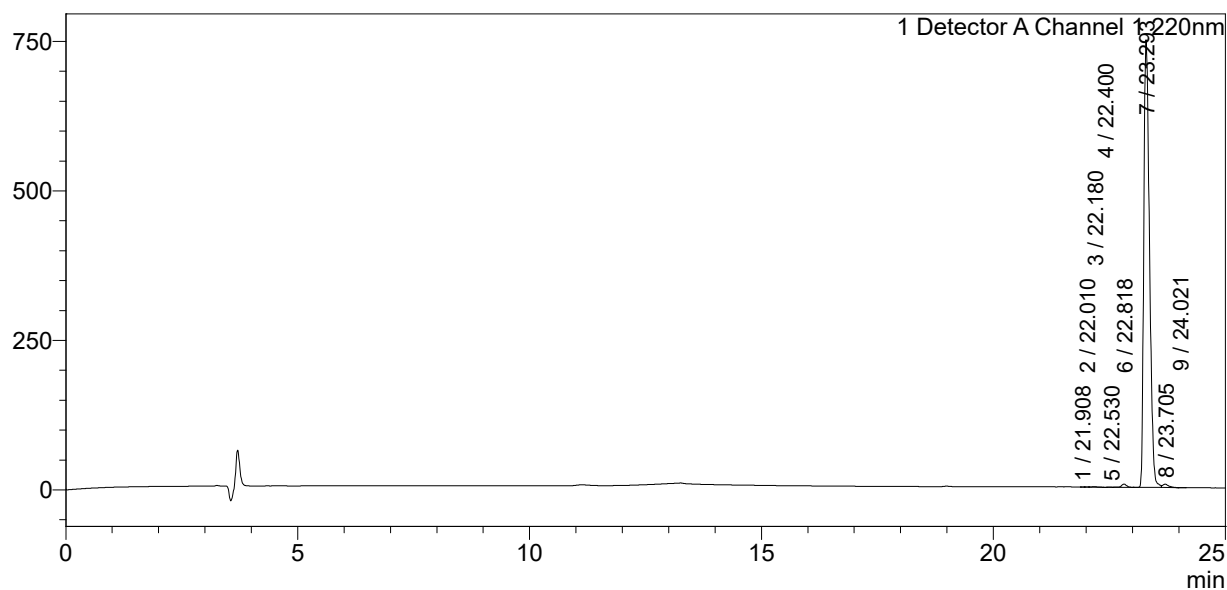

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	21.908	85	29	0.001
2	22.010	301	78	0.005
3	22.180	5796	753	0.089
4	22.400	107	33	0.002
5	22.530	759	125	0.012
6	22.818	41633	5508	0.641
7	23.293	6395935	748681	98.467
8	23.705	50462	5733	0.777
9	24.021	402	74	0.006
Total		6495479	761014	100.000