


Mass Spectrum

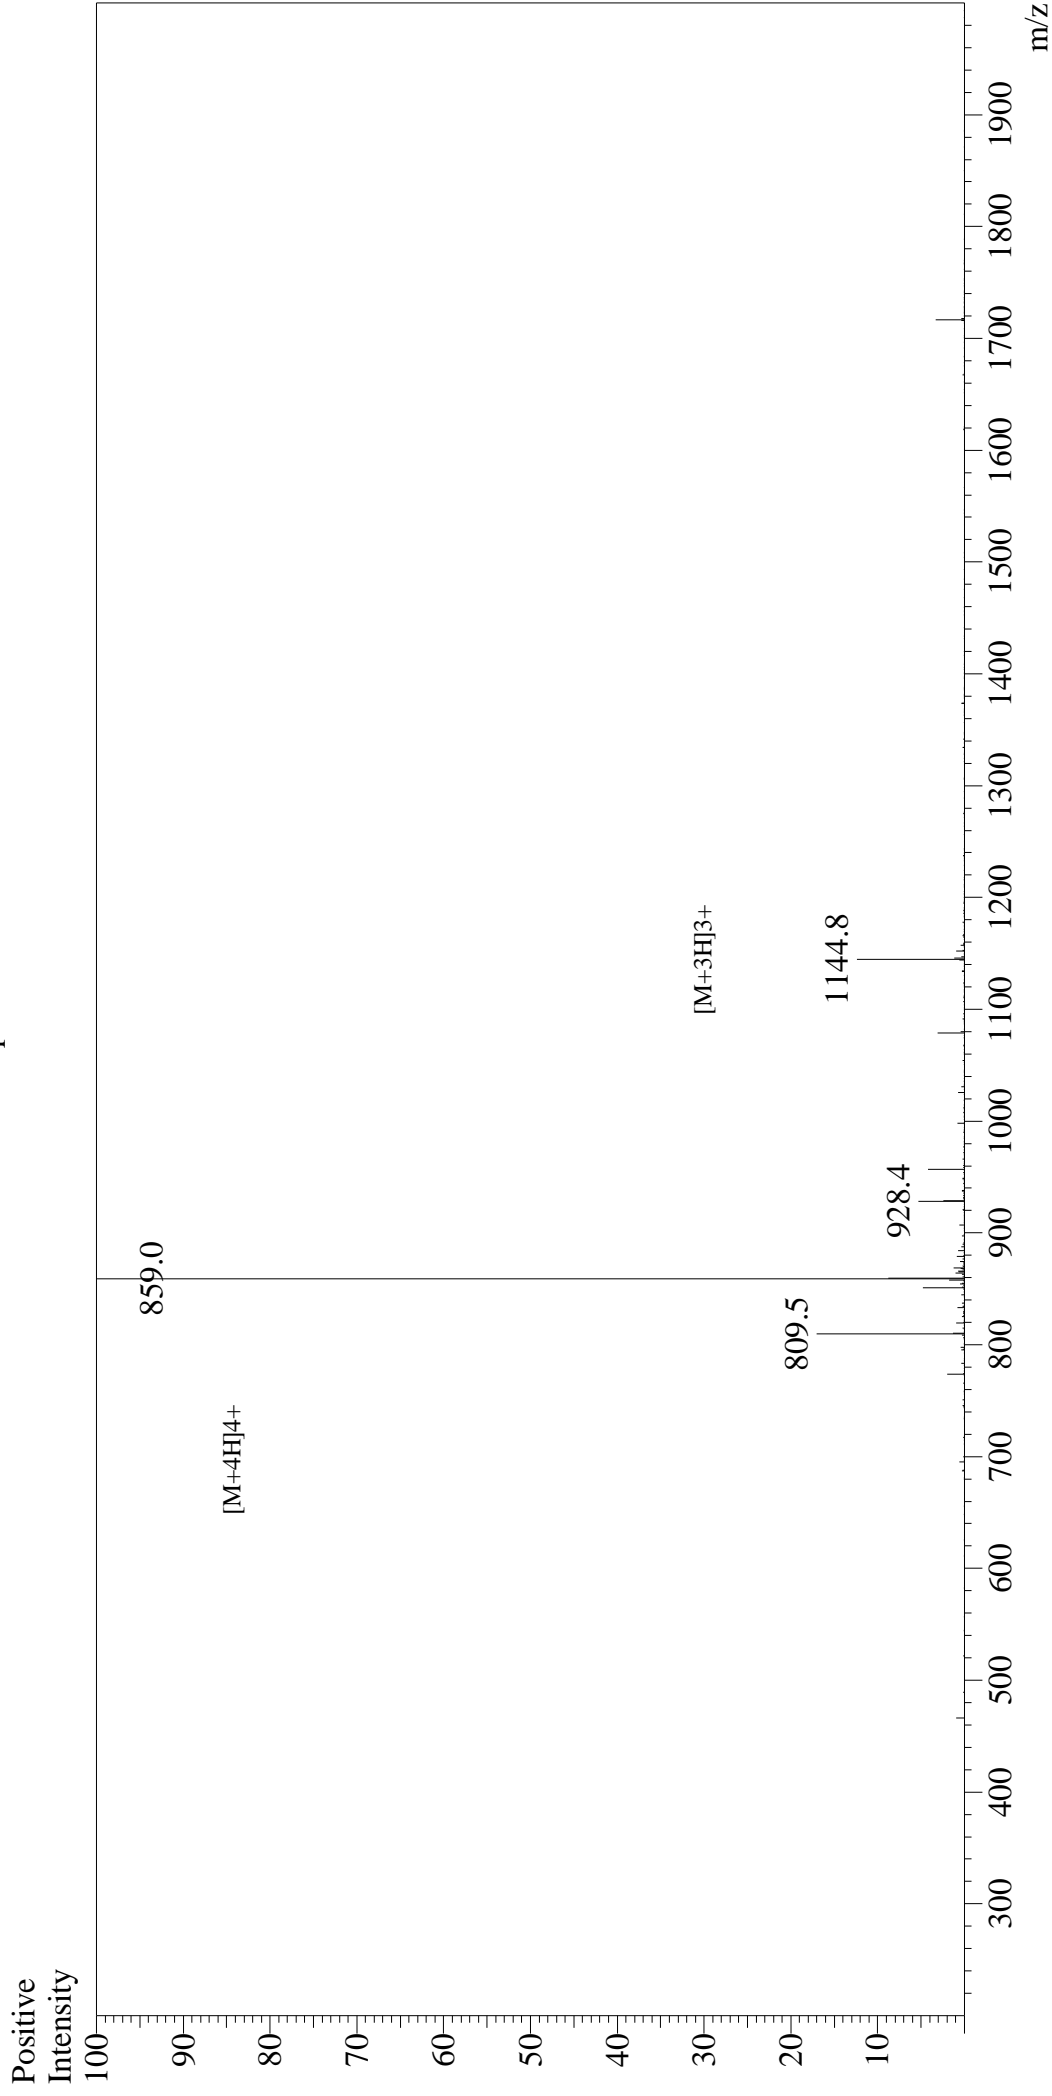

Sample Information

User : Gary
Month-Day Processed : 10/07/18
Time Processed : 16:15:19
Injection Volume : 0.2
Sample Name : Calcitonin, salmon
Cat No. : RP11099
Lot No. : PE2871809
Theoretical MW : 3431.90
Observed MW : 3432.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH