


Mass Spectrum

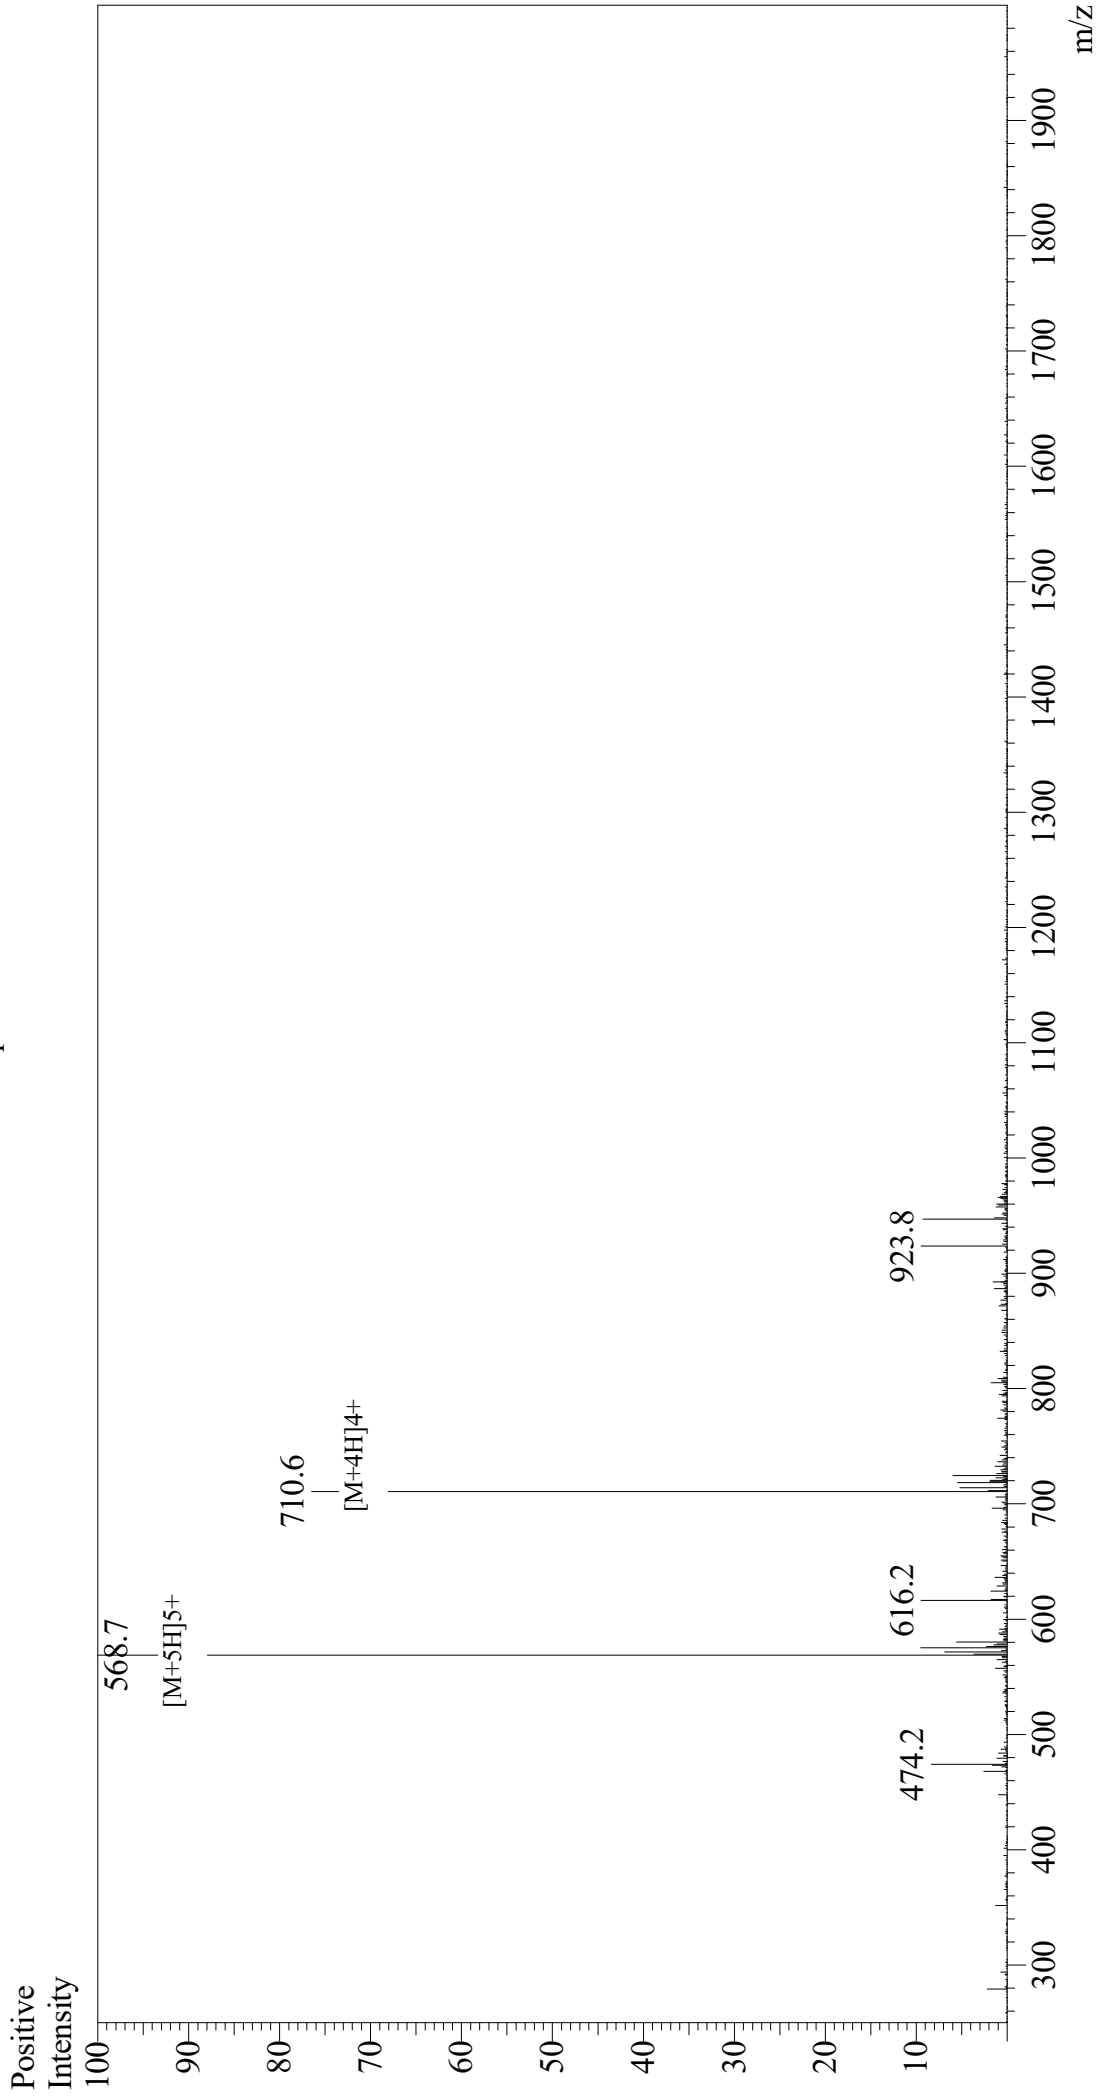

Sample Information

Month-Day/Processed : 01/27/21
Time Processed : 4:22:15 AM
Injection Volume : 0.6
Sample Name : BAM-22P
Cat No. : RP10424
Lot No. : E0631821A
Theoretical MW : 2839.23
Observed MW : 2838.5

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH