

Sample Name :DYKDDDDK Peptide  
 Cat No. :RP10586  
 Lot No. :E2600321A  
 Time Processed :4:12:21 PM  
 Month-Day-Year Processed :01/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

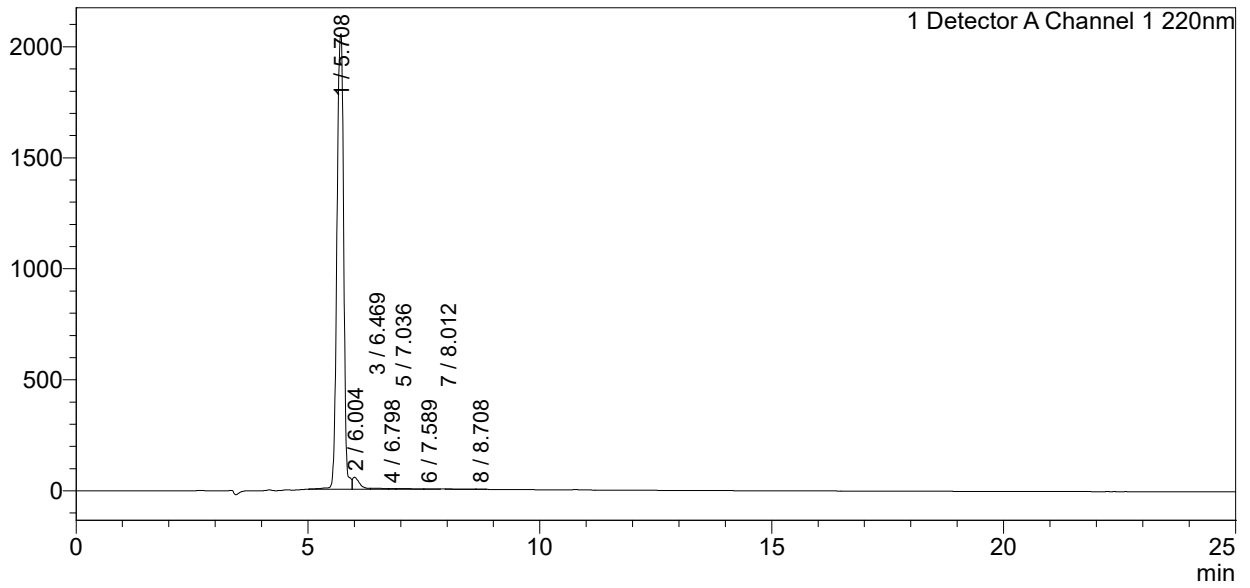

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.708	20524770	2051778	96.186
2	6.004	563376	54514	2.640
3	6.469	87587	4539	0.410
4	6.798	26885	3014	0.126
5	7.036	82524	3266	0.387
6	7.589	27229	1556	0.128
7	8.012	19775	1026	0.093
8	8.708	6528	1136	0.031
Total		21338675	2120830	100.000