

Sample Name :CLIP (86-100)
 Cat No. :RP20279
 Lot No. :E9431520B
 Time Processed :11:23:04
 Month-Day-Year Processed :02/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

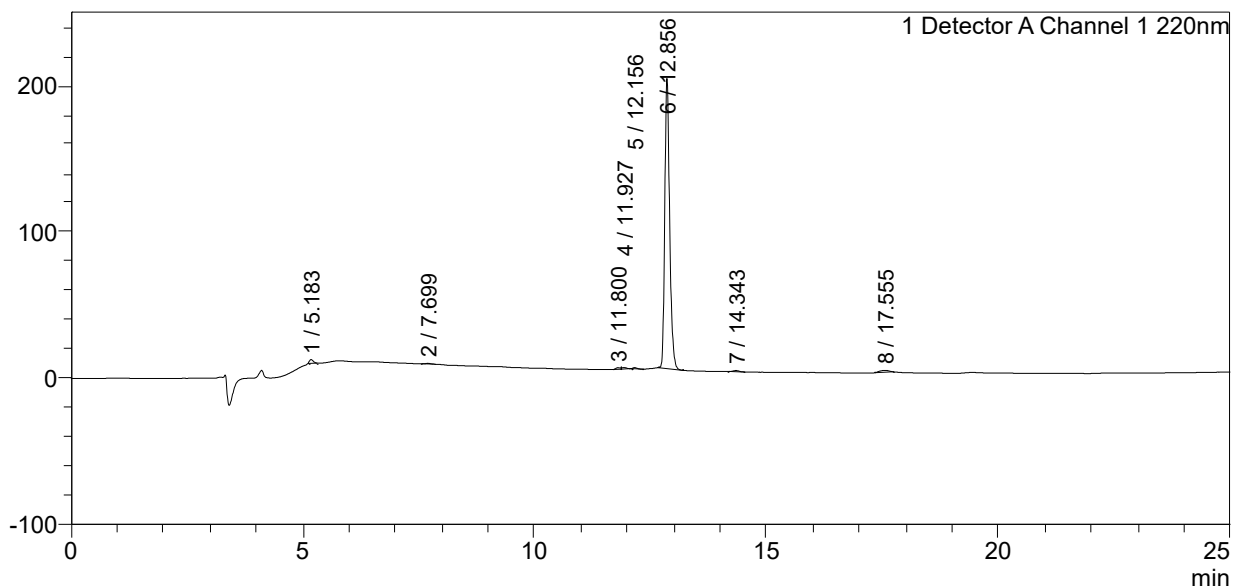

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.183	14066	2500	0.931
2	7.699	2978	479	0.197
3	11.800	6788	1071	0.449
4	11.927	7445	1052	0.493
5	12.156	4602	853	0.304
6	12.856	1449706	198062	95.923
7	14.343	7011	808	0.464
8	17.555	18720	1285	1.239
Total		1511317	206111	100.000