

Sample Name :43Gap 26, Connexin Mimetic
 Cat. No. : RP20274
 Lot. No. : PE4731810
 Time Processed : 9:30:59
 Month-Day-Year Processed : 11/02/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

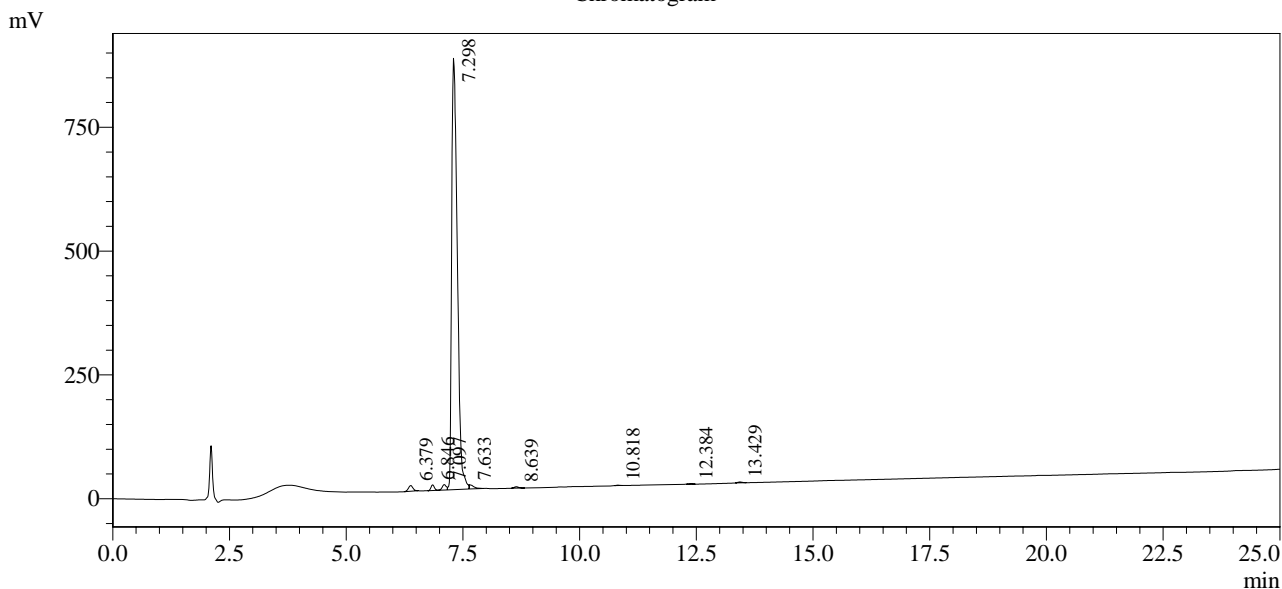

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.379	76142	11383	0.997
2	6.846	58535	11408	0.766
3	7.097	67231	11054	0.880
4	7.298	7344458	871065	96.149
5	7.633	55704	8420	0.729
6	8.639	19090	2787	0.250
7	10.818	3911	799	0.051
8	12.384	2873	486	0.038
9	13.429	10651	1702	0.139
Total		7638596	919104	100.000