

Sample Name : VIP, human, ovine, porcine, rat  
 Cat. No. : RP10085  
 Lot. No. : 16018007590016/PE3020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

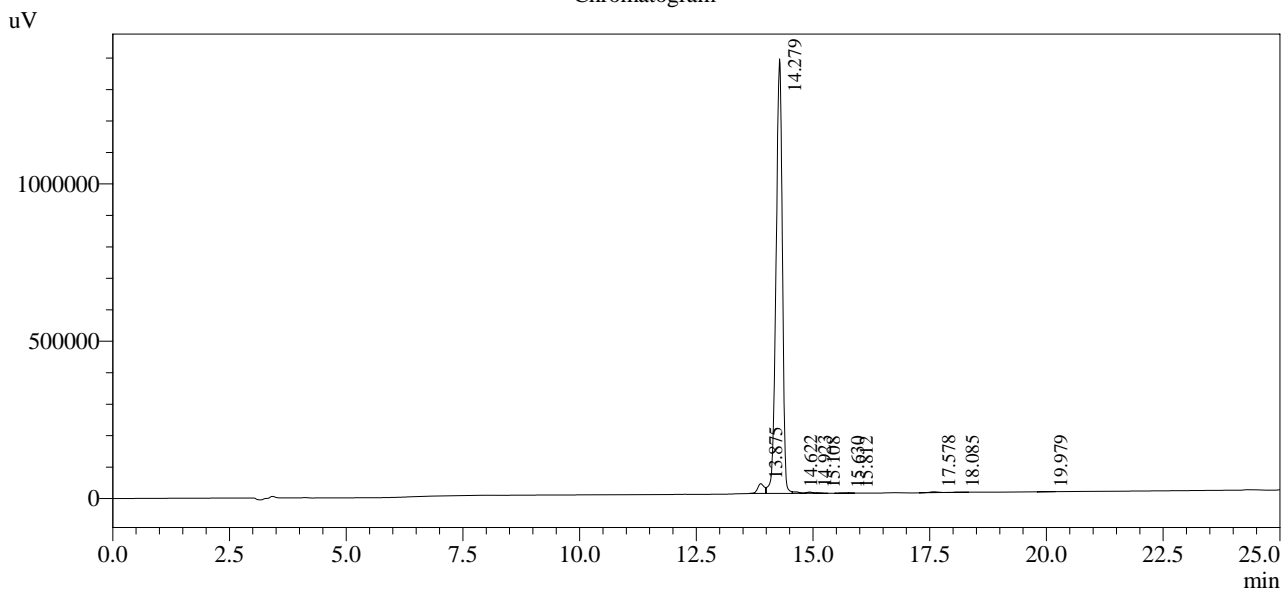

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.875	307254	30965	2.293
2	14.279	12947165	1381125	96.621
3	14.622	45242	5023	0.338
4	14.923	38036	3836	0.284
5	15.108	7549	1137	0.056
6	15.630	4346	461	0.032
7	15.812	592	107	0.004
8	17.578	33068	2704	0.247
9	18.085	10839	1093	0.081
10	19.979	5869	546	0.044
Total		13399959	1426996	100.000