

Sample Name: OVA G4 peptide  
 Cat No. : RP20398  
 Lot No. : E2676221D  
 Time Processed : 1:11:02 AM  
 Month-Day-Year Processed : 04/15/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

<Chromatogram>

mV

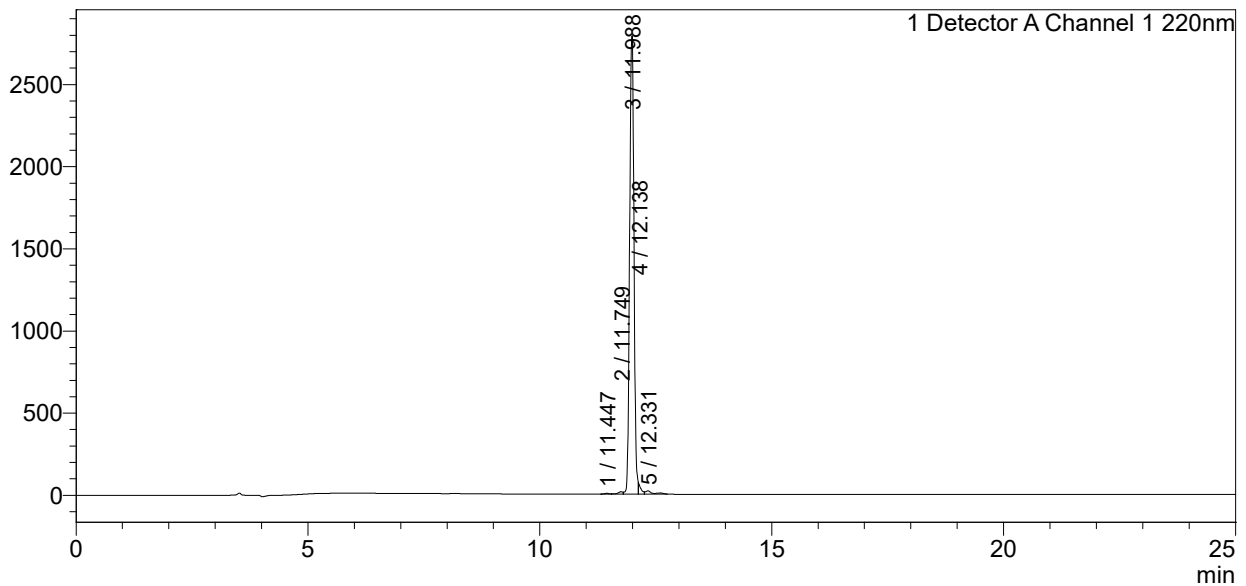

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.447	23598	4294	0.126
2	11.749	98513	14128	0.526
3	11.988	18169336	2790699	96.949
4	12.138	237770	64118	1.269
5	12.331	211999	19093	1.131
Total		18741216	2892331	100.000