

Sample Name : Nuclear Localiation Signal Peptide
 Cat No.: RP20292
 Lot No.: E5422120F
 Time Processed : 9:37:32
 Month-Day-Year Processed : 06/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	0
40.00	Pumps	Pump A B.Conc	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

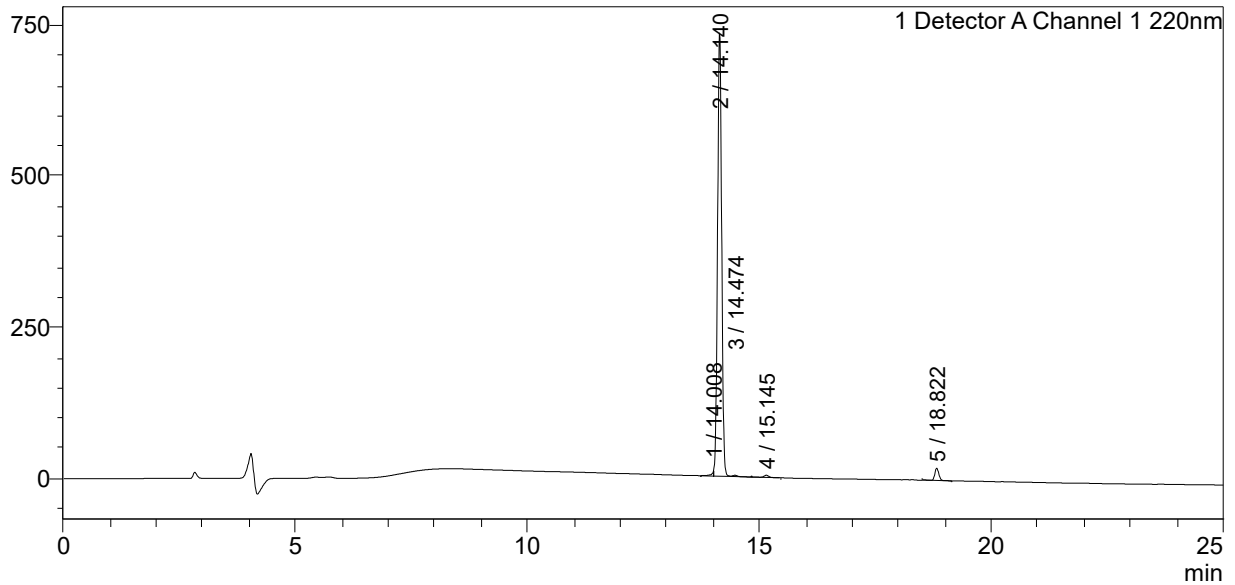

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.008	29096	7446	0.616
2	14.140	4530162	732943	95.969
3	14.474	16218	2273	0.344
4	15.145	24982	3669	0.529
5	18.822	119987	20227	2.542
Total		4720444	766558	100.000