

Sample Name : (Arg)9
 Cat No. : RP20403
 Lot No. : E4942619I
 Time Processed : 10:13:01
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010507

<Chromatogram>

mV

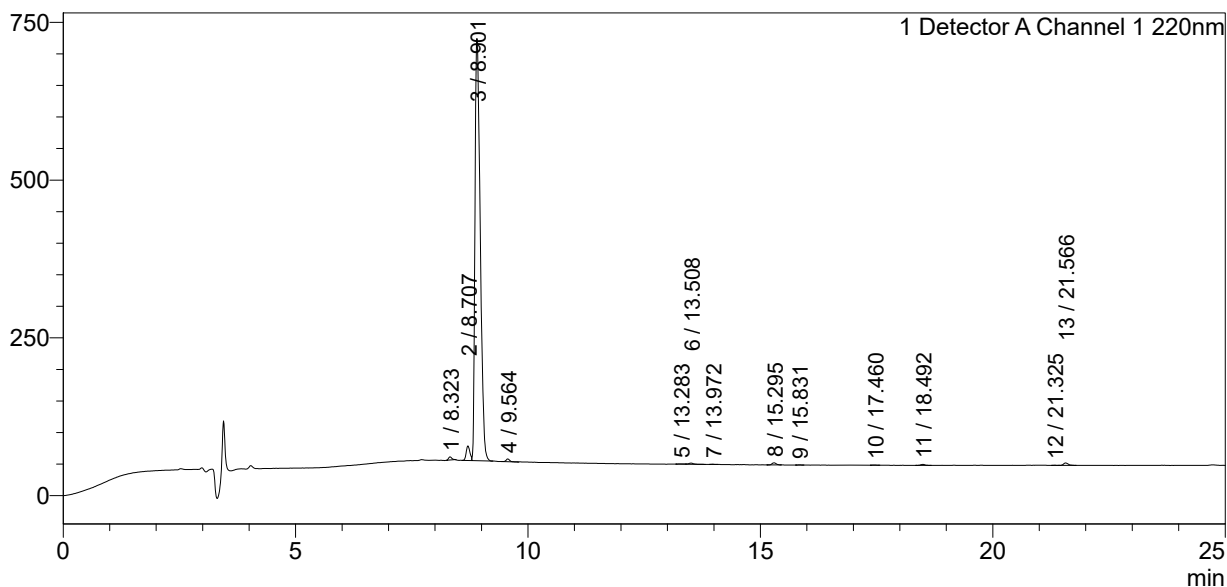

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.323	24059	4951	0.438
2	8.707	129250	23257	2.351
3	8.901	5234037	668953	95.193
4	9.564	24357	4458	0.443
5	13.283	4498	465	0.082
6	13.508	16159	1944	0.294
7	13.972	1930	435	0.035
8	15.295	20816	3293	0.379
9	15.831	1441	267	0.026
10	17.460	2553	405	0.046
11	18.492	9624	1472	0.175
12	21.325	1202	244	0.022
13	21.566	28397	3991	0.516
Total		5498325	714135	100.000