

Sample Name : RGD  
 Cat. No. : RP20297  
 Lot. No. : E4862019I  
 Time Processed : 13:29:04  
 Month-Day-Year Processed : 09/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

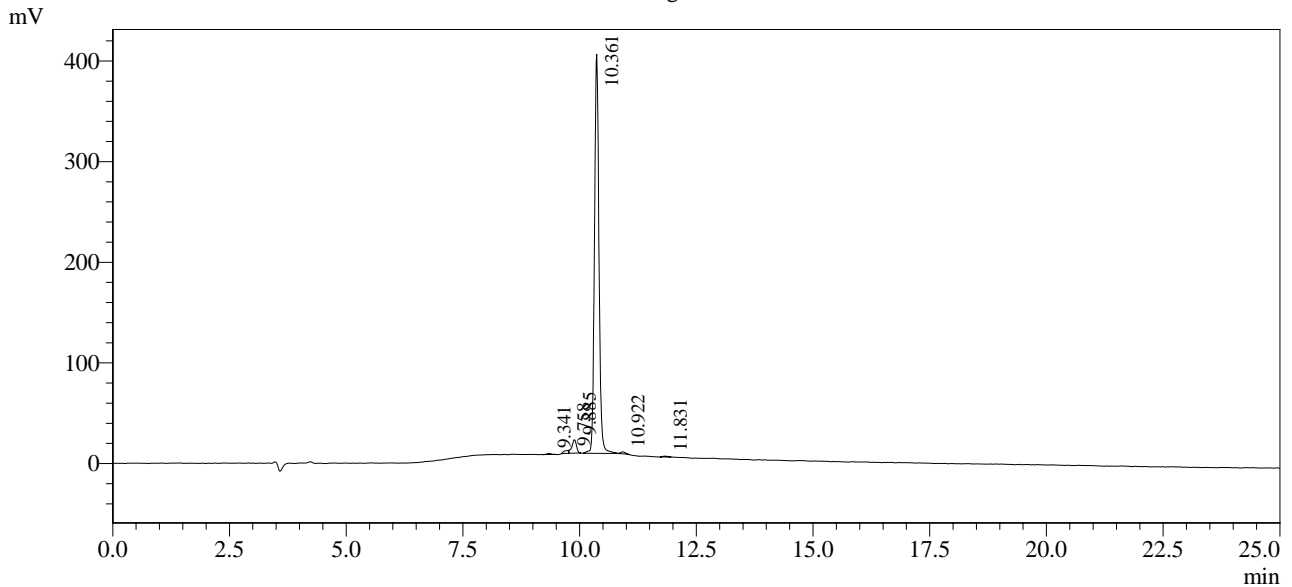

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.341	6974	1151	0.251
2	9.758	20704	2929	0.744
3	9.885	90310	13346	3.244
4	10.361	2647103	396609	95.100
5	10.922	13058	1938	0.469
6	11.831	5359	786	0.193
Total		2783508	416759	100.000