

Sample Name :[Leu5]-Enkephalin  
 Cat No. :RP10884  
 Lot No. :E4771419I  
 Time Processed :1:35:06  
 Month-Day-Year Processed :09/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

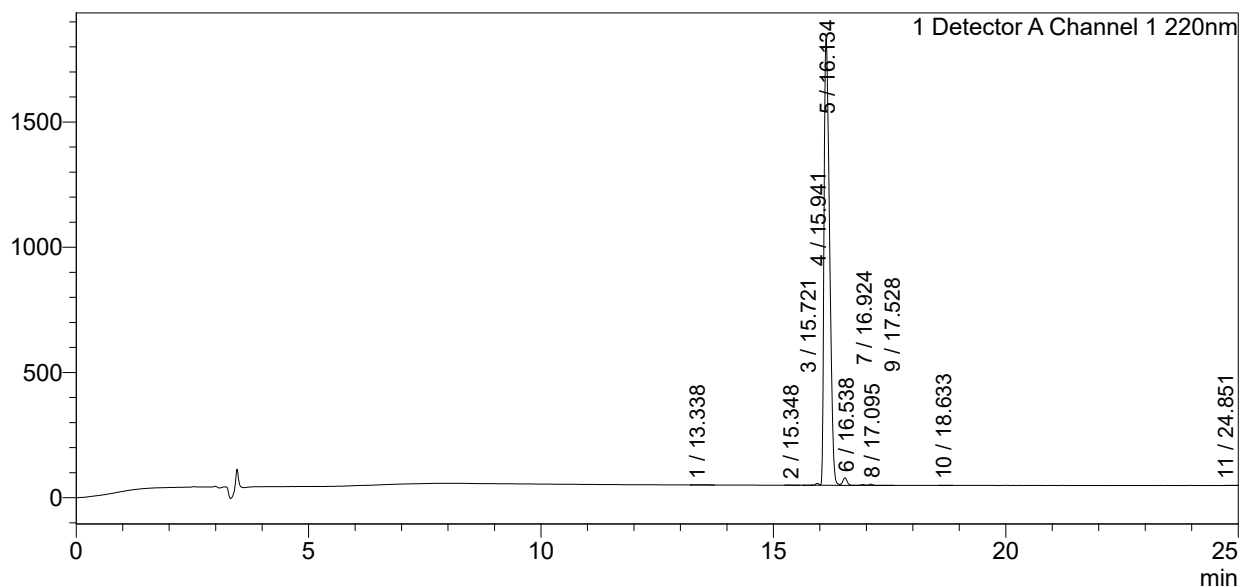

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.338	7164	420	0.048
2	15.348	6181	797	0.041
3	15.721	2814	454	0.019
4	15.941	39532	7398	0.263
5	16.134	14730780	1783584	97.990
6	16.538	193779	30088	1.289
7	16.924	16911	2931	0.112
8	17.095	27210	4443	0.181
9	17.528	1868	205	0.012
10	18.633	1524	198	0.010
11	24.851	5232	515	0.035
Total		15032996	1831032	100.000