

Sample Name :[Glu1]-Fibrinopeptide B
 Cat No. :RP20439
 Lot No. :E2664420L
 Time Processed :8:08:12
 Month-Day-Year Processed :12/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

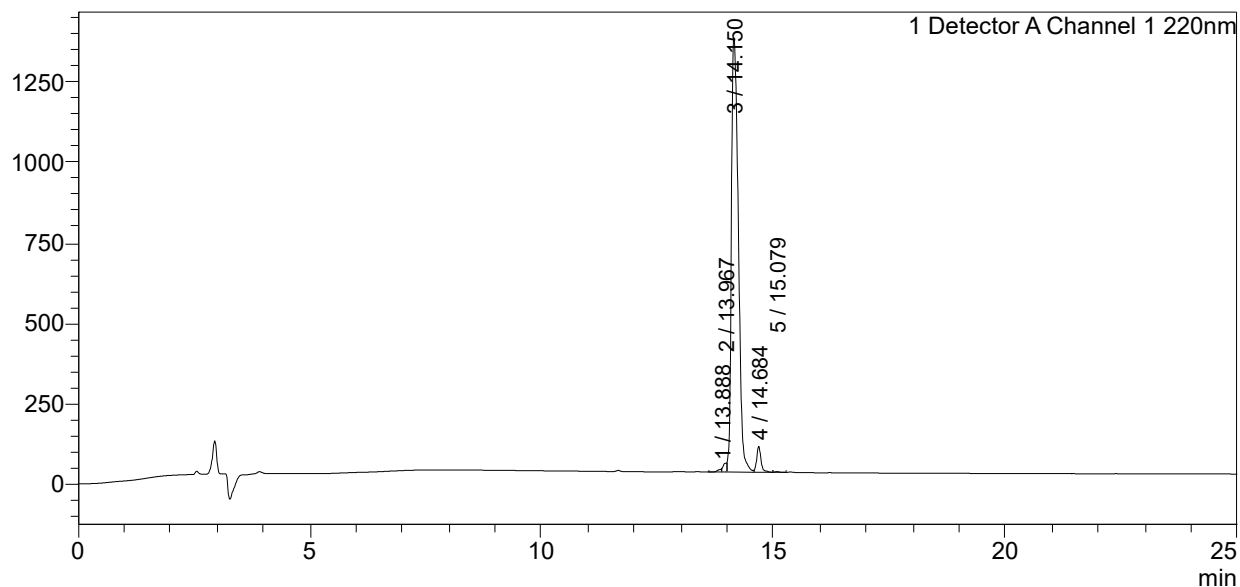

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.888	58330	10052	0.395
2	13.967	114205	27460	0.773
3	14.150	14071044	1351844	95.190
4	14.684	524626	80506	3.549
5	15.079	13807	2264	0.093
Total		14782011	1472126	100.000