

Sample Name : Proctolin  
 Cat. No. : RP10475  
 Lot. No. : PE7981707


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

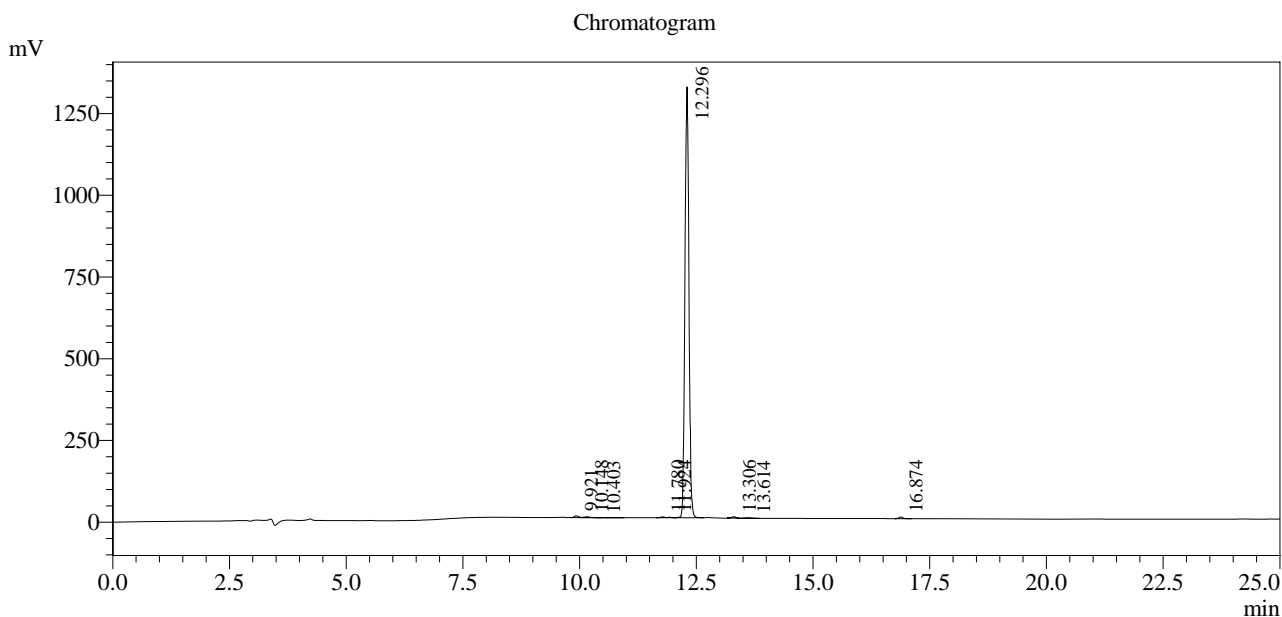

I Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.921	38538	5331	0.479
2	10.148	24207	2935	0.301
3	10.403	6680	553	0.083
4	11.780	19049	2751	0.237
5	11.924	9899	1875	0.123
6	12.296	7881695	1318388	97.954
7	13.306	27344	4188	0.340
8	13.614	9019	1126	0.112
9	16.874	29872	5064	0.371
Total		8046305	1342212	100.000