

Sample Name :Fibronectin Active Fragment Control
Cat No. :RP20347
Lot No. :E4962619I
Time Processed :8:25:38
Month-Day-Year Processed :09/23/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

<Chromatogram>

mV

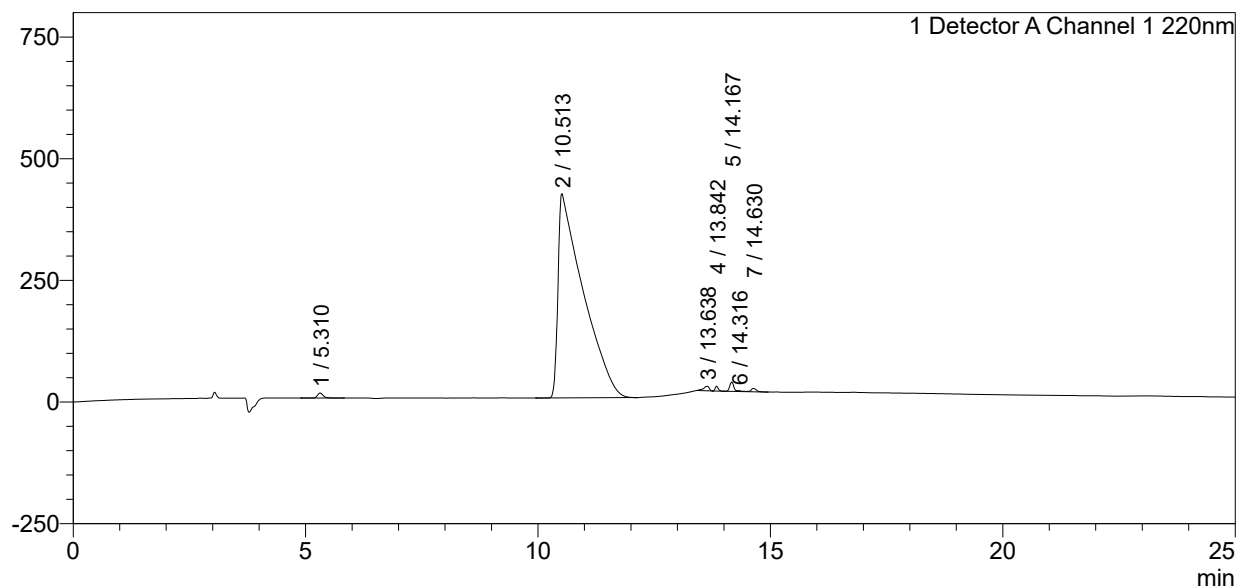

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.310	88104	10335	0.547
2	10.513	15706219	419563	97.529
3	13.638	80607	9225	0.501
4	13.842	47619	10117	0.296
5	14.167	114991	19410	0.714
6	14.316	9817	1829	0.061
7	14.630	56735	6816	0.352
Total		16104092	477294	100.000