


# Mass Spectrum

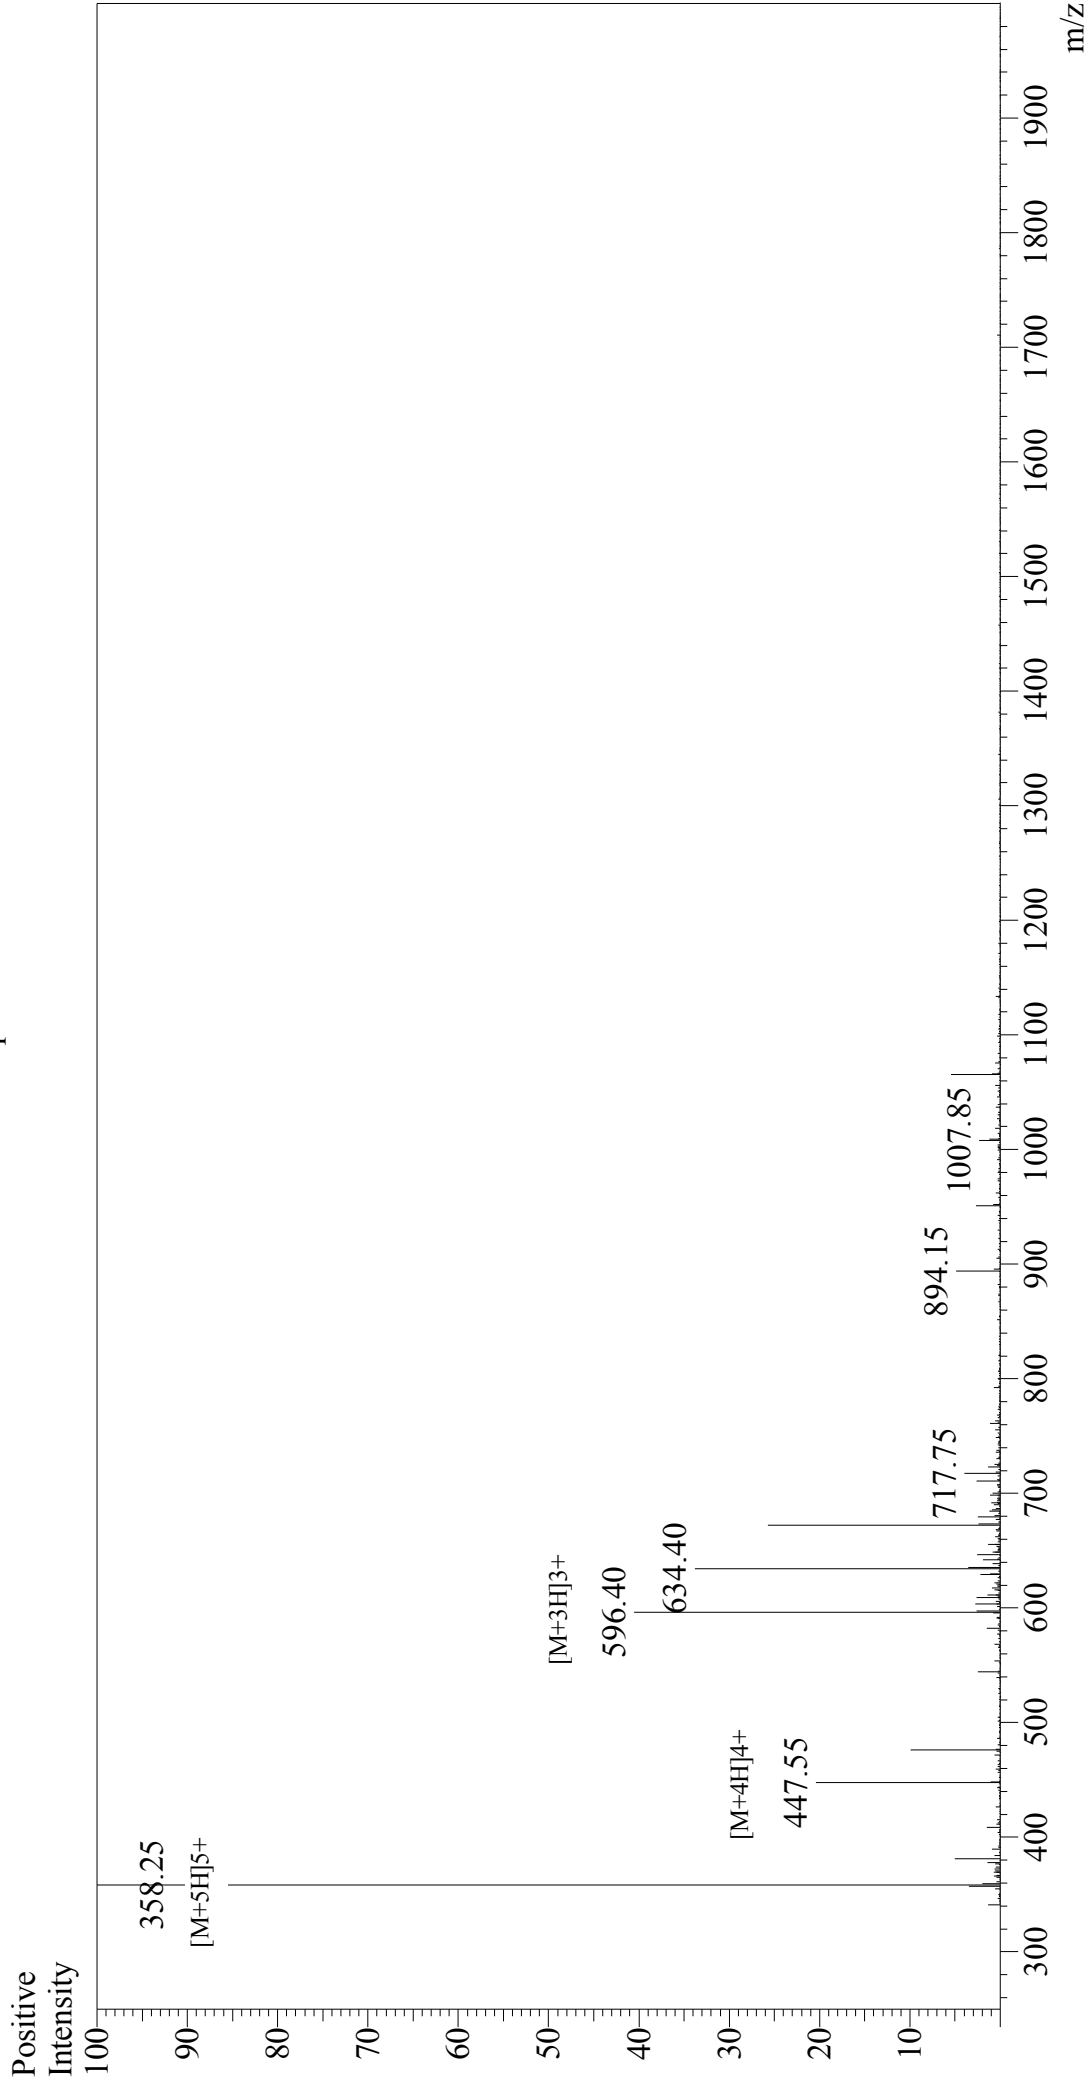

## Sample Information

Acquired by : Gary  
Month-Day Processed : 12/30/17  
Time Processed : 13:15:35  
Injection Volume : 0.2  
Sample Name : Biotin-TAT (47-57)  
Cat.No. : RP20408  
Lot.No : PE2451712  
Theoretical MW : 1786.20  
Observed MW : 1786.25

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250°C  
Block Temp : 200°C

Interface Bias : +4.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50% H<sub>2</sub>O/50% MeOH