

Sample Name: β -Amyloid (1-42), human
 Cat No. : RP10017
 Lot No. :E6123820J
 Time Processed: 20:45:21
 Month-Day-Year Processed :11/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	10
25.00	Pumps	Solvent B Conc.	100
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	10
35.00	Pumps	Solvent B Conc.	10
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

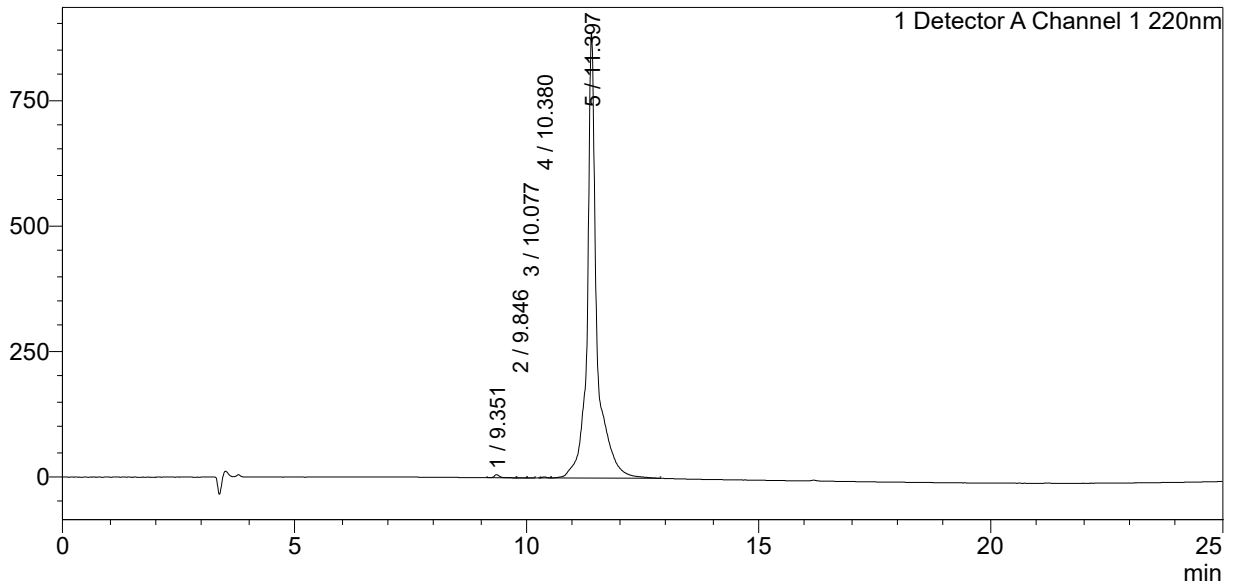

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.351	47711	6155	0.375
2	9.846	1542	208	0.012
3	10.077	1392	194	0.011
4	10.380	15351	2298	0.121
5	11.397	12664071	884790	99.482
Total		12730068	893646	100.000