


Mass Spectrum

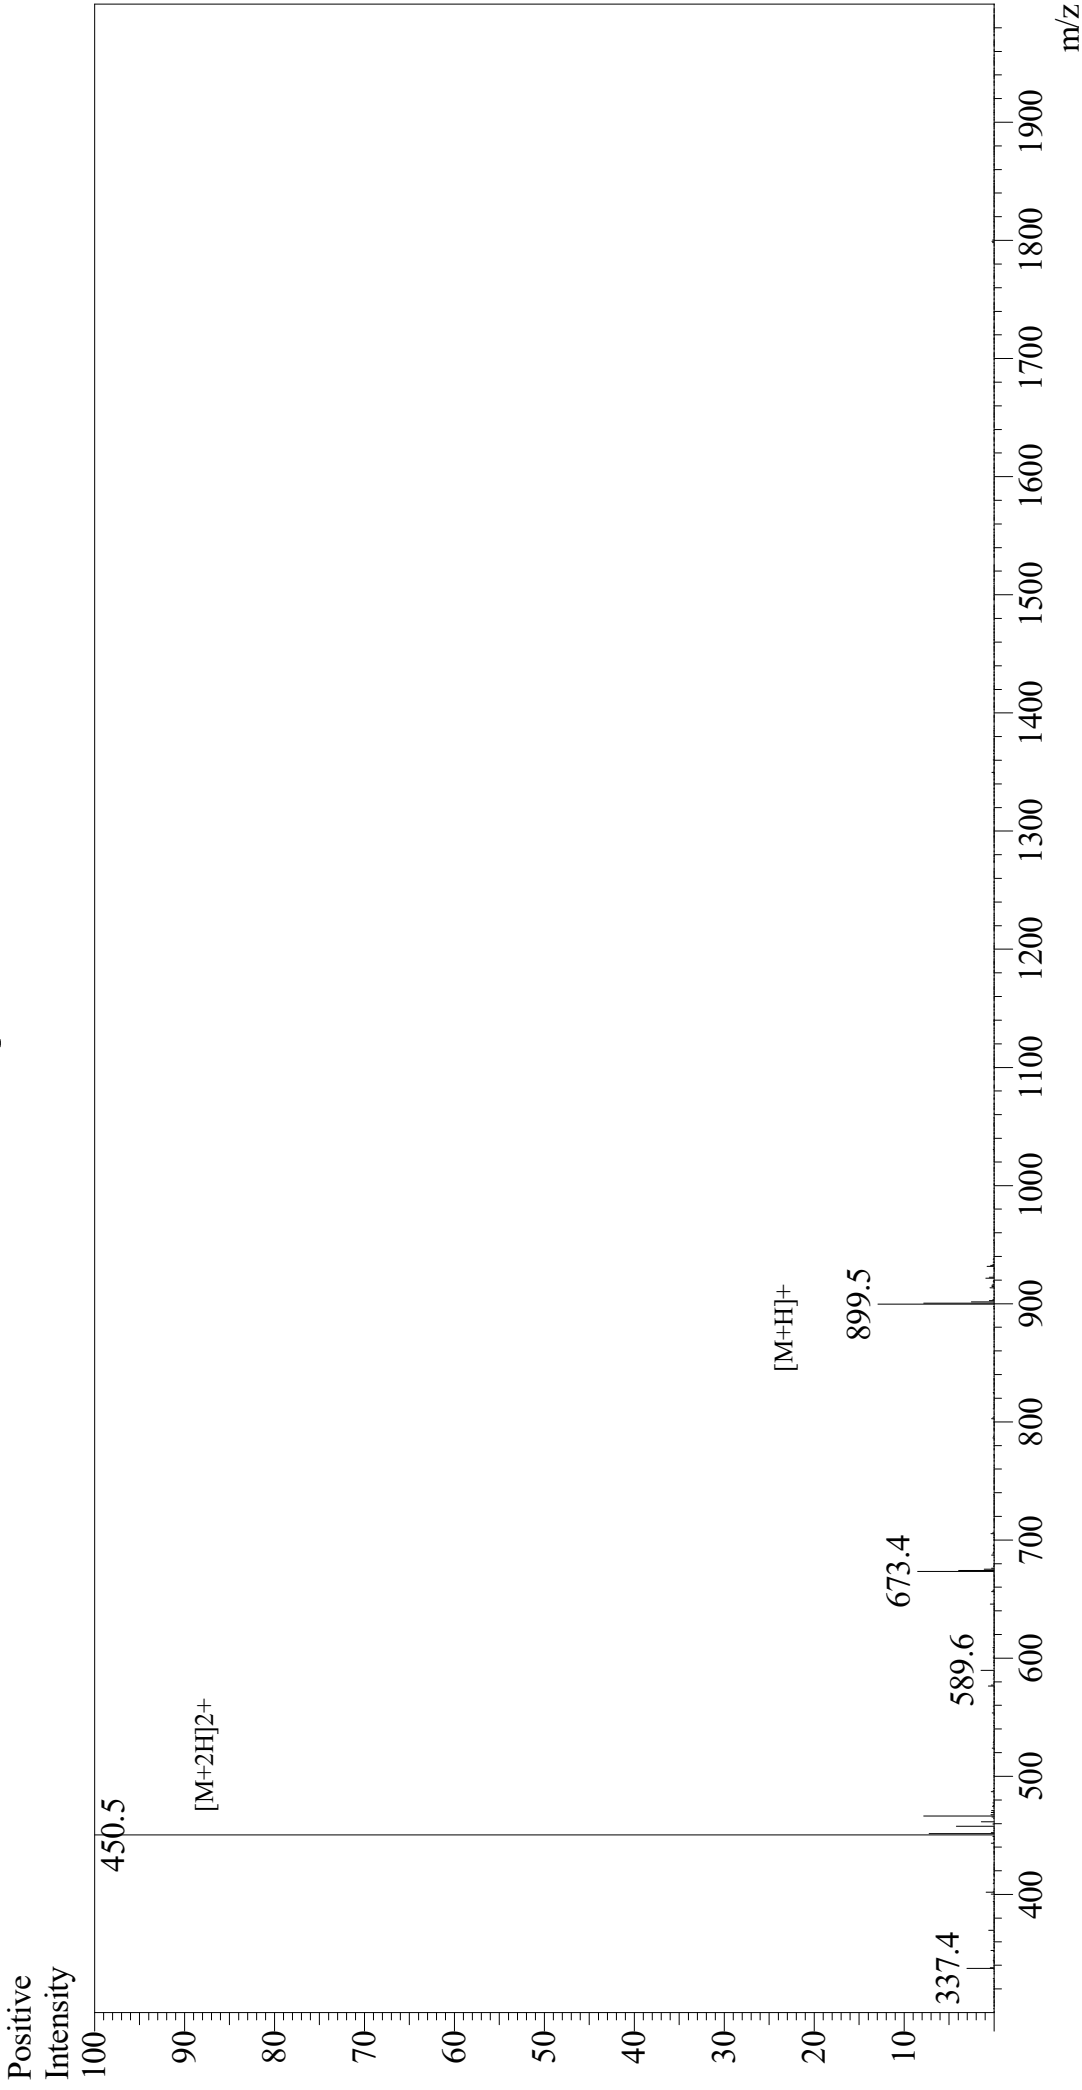

Sample Information

Acquired by: Gary
Month-Day Processed: 11/16/19
Time Processed: 08:43:02 AM
Injection Volume: 0.3
Sample Name: Cardiotoxin Analog (CTX) IV (6-12)
Cat. No.: RP17303
Lot. No.: E6871619K
Theoretical MW: 899.14
Observed MW: 899.0

Interface: ESI
Nebulizing Gas Flow: 1.5L/min
CDL Temp: 250
Block Temp: 200

Equipment: GK11010007
Interface Bias: +4.5 kV
Drying Gas Flow: 5 L/min
T.Flow: 0.2 ml/min
B.conc: 50% H₂O/50% MeOH