

Sample Name :[Asp371]-Tyrosinase (369-377), human
 Cat No. :RP10270
 Lot No. :E6648621G
 Time Processed :2:16:51 AM
 Month-Day-Year Processed :07/03/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

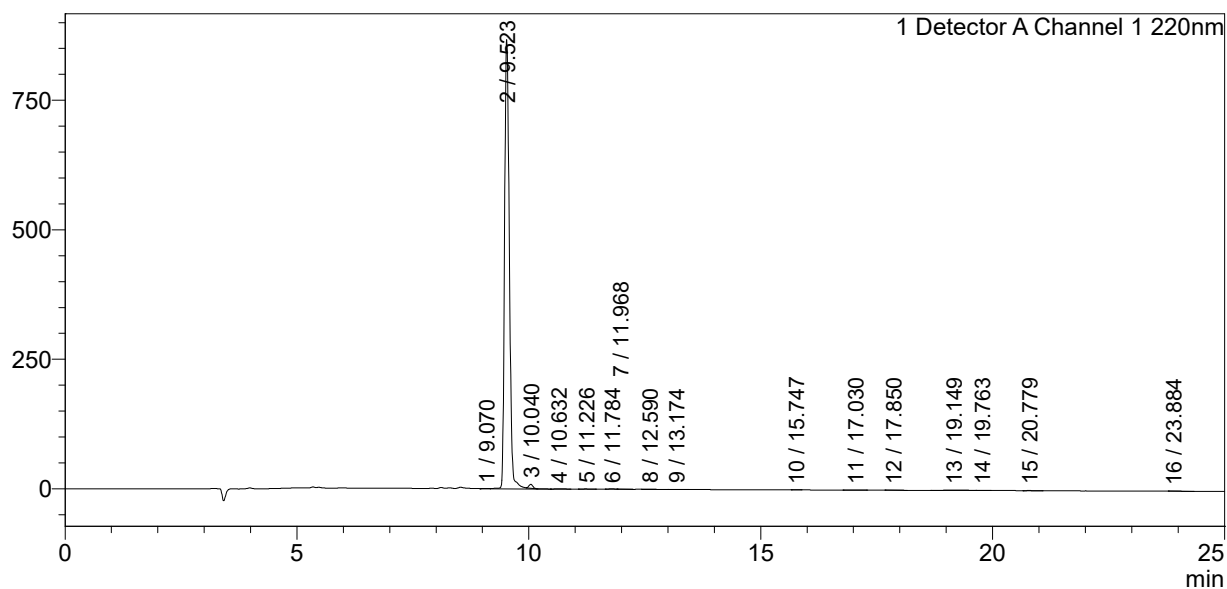

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.070	3573	453	0.057
2	9.523	6191108	867195	98.290
3	10.040	43649	7595	0.693
4	10.632	3640	421	0.058
5	11.226	2781	282	0.044
6	11.784	7886	1134	0.125
7	11.968	3698	395	0.059
8	12.590	6824	377	0.108
9	13.174	3185	268	0.051
10	15.747	1299	164	0.021
11	17.030	4490	271	0.071
12	17.850	2904	179	0.046
13	19.149	18664	570	0.296
14	19.763	1309	127	0.021

Peak#	Ret. Time	Area	Height	Area%
15	20.779	2602	244	0.041
16	23.884	1197	90	0.019
Total		6298807	879765	100.000