

Sample Name :Angiotensinogen (1-14), human
 Cat No. :RP10253
 Lot No. :E4709619I
 Time Processed :19:50:32
 Month-Day-Year Processed :09/24/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

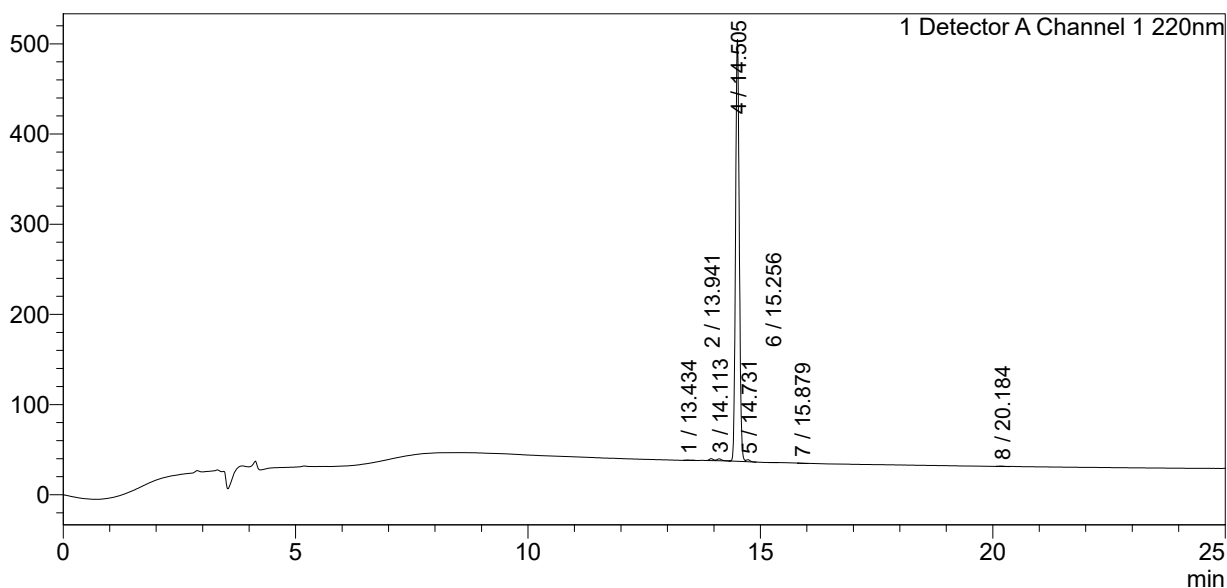

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.434	3562	391	0.134
2	13.941	12351	2149	0.465
3	14.113	14265	2097	0.537
4	14.505	2609398	467781	98.158
5	14.731	13126	2335	0.494
6	15.256	1388	311	0.052
7	15.879	1768	343	0.067
8	20.184	2510	366	0.094
Total		2658368	475774	100.000