

Sample Name :Hexa-His
 Cat. No. : RP11737
 Lot. No. : PE8431902
 Time Processed :20:39:19
 Month-Day-Year Processed : 03/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	1	
25.00	Pumps	Pump A B.Conc	50	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	1	
40.00	Pumps	Pump A B.Conc	1	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

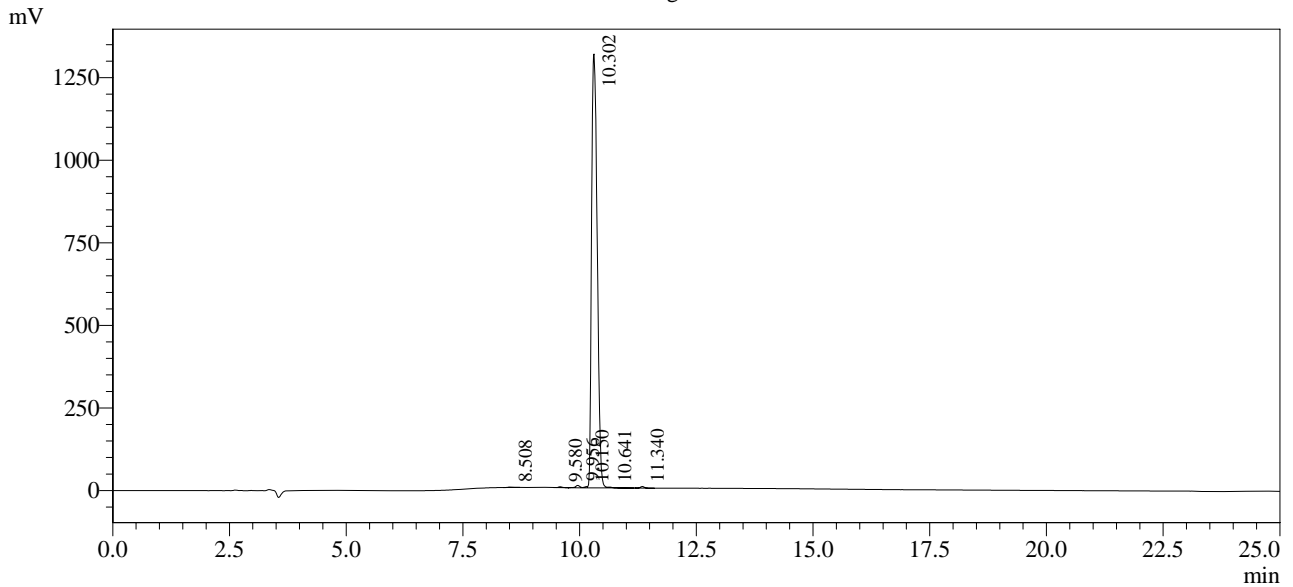

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.508	9450	1525	0.085
2	9.580	15878	2641	0.142
3	9.956	46361	7107	0.415
4	10.150	15552	3531	0.139
5	10.302	11047760	1313909	98.798
6	10.641	17944	2704	0.160
7	11.340	29265	4954	0.262
Total		11182209	1336370	100.000