

SampleName: Arg-Gly-Asp-Cys
 Cat No.: RP10860
 Lot No.: E4777019J
 Time Processed :8:45:14 AM
 Month-Day-Year Processed :11/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

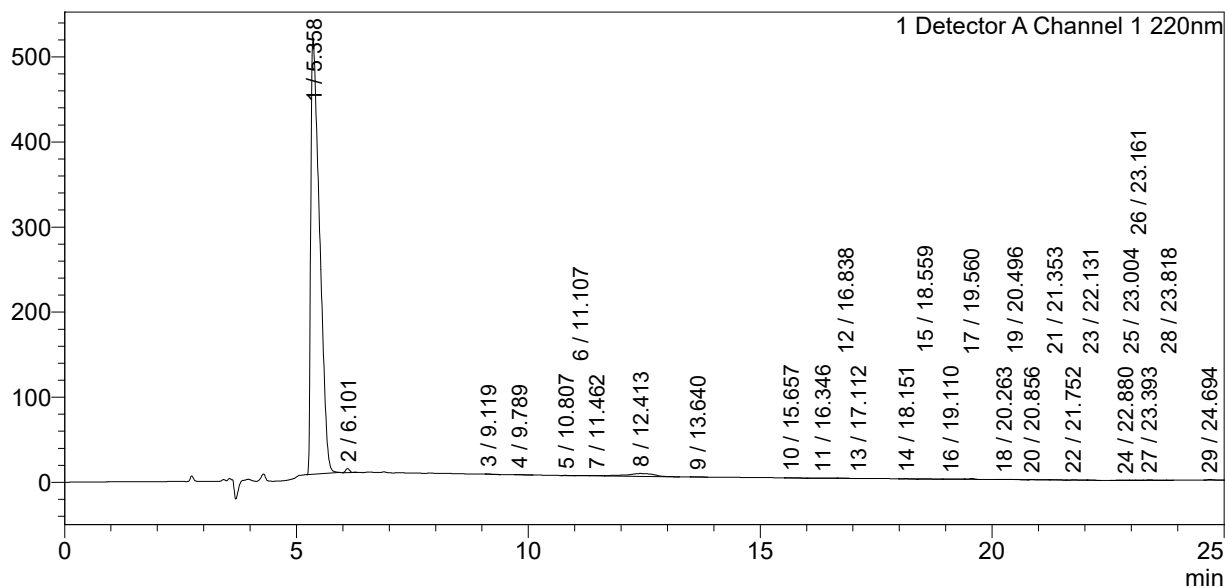

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.358	6788812	512856	96.382
2	6.101	27536	4818	0.391
3	9.119	1343	76	0.019
4	9.789	1669	85	0.024
5	10.807	1017	127	0.014
6	11.107	1388	162	0.020
7	11.462	5156	336	0.073
8	12.413	141654	3386	2.011
9	13.640	1402	134	0.020
10	15.657	3748	205	0.053
11	16.346	5842	297	0.083
12	16.838	2136	244	0.030
13	17.112	1387	66	0.020
14	18.151	3326	288	0.047
15	18.559	5116	329	0.073

Peak#	Ret. Time	Area	Height	Area%
16	19.110	4160	275	0.059
17	19.560	7256	1106	0.103
18	20.263	1353	156	0.019
19	20.496	1168	101	0.017
20	20.856	4737	477	0.067
21	21.353	1146	95	0.016
22	21.752	2021	148	0.029
23	22.131	1455	141	0.021
24	22.880	5381	280	0.076
25	23.004	1945	260	0.028
26	23.161	2142	249	0.030
27	23.393	9884	697	0.140
28	23.818	1083	133	0.015
29	24.694	8400	863	0.119
Total		7043664	528390	100.000