

Sample Name :Beta-Amyloid (35-25)
 Cat No.: RP20185
 Lot No.: PE5091905
 Time Processed :14:05:47
 Month-Day-Year Processed :05/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
25.00	Pumps	Solvent B Conc.	60
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010509

<Chromatogram>

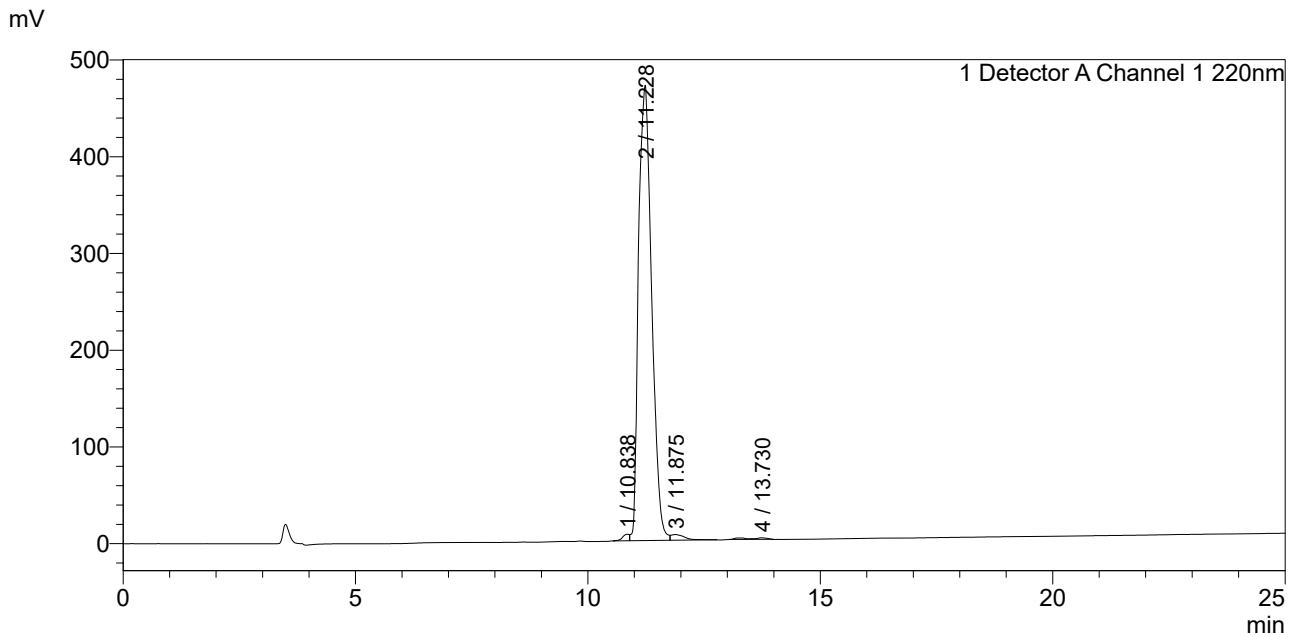

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.838	67609	6636	0.715
2	11.228	9212673	470570	97.445
3	11.875	119860	5887	1.268
4	13.730	54050	1609	0.572
Total		9454192	484702	100.000