

Sample Name : RGD
 Cat. No. :RP20297
 Lot. No. :PE2371805


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

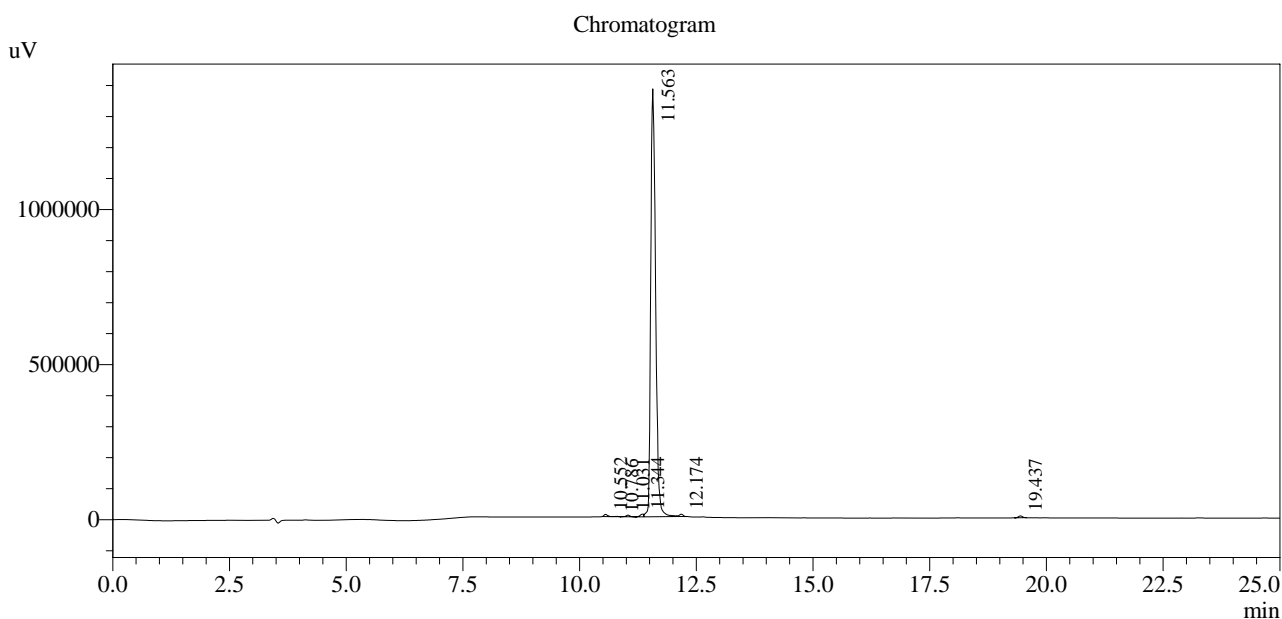

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.552	37080	6940	0.361
2	10.786	6136	1161	0.060
3	11.031	30436	5221	0.297
4	11.344	45656	8615	0.445
5	11.563	10064399	1379719	98.066
6	12.174	43237	7396	0.421
7	19.437	35917	6140	0.350
Total		10262862	1415192	100.000