

Sample Name :SV40 large T antigen NLS

Cat. No. : RP20414

Lot. No. : E8656920K

Time Processed :12:27:37 AM

Month-Day-Year Processed :11/12/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	15
25.00	Pumps	B.Conc	75
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	15
40.00	Pumps	B.Conc	15
41.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010140

<Chromatogram>

mV

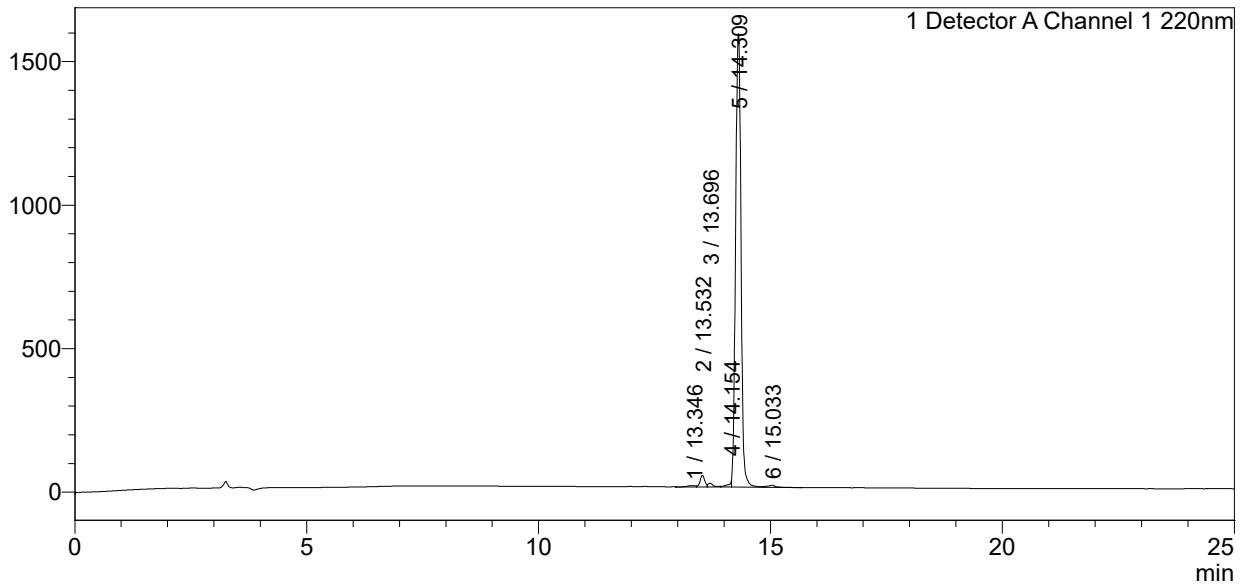

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.346	50723	4230	0.378
2	13.532	281042	40825	2.093
3	13.696	106511	13074	0.793
4	14.154	102068	18351	0.760
5	14.309	12796725	1580304	95.294
6	15.033	91606	7234	0.682
Total		13428675	1664017	100.000