


Mass Spectrum

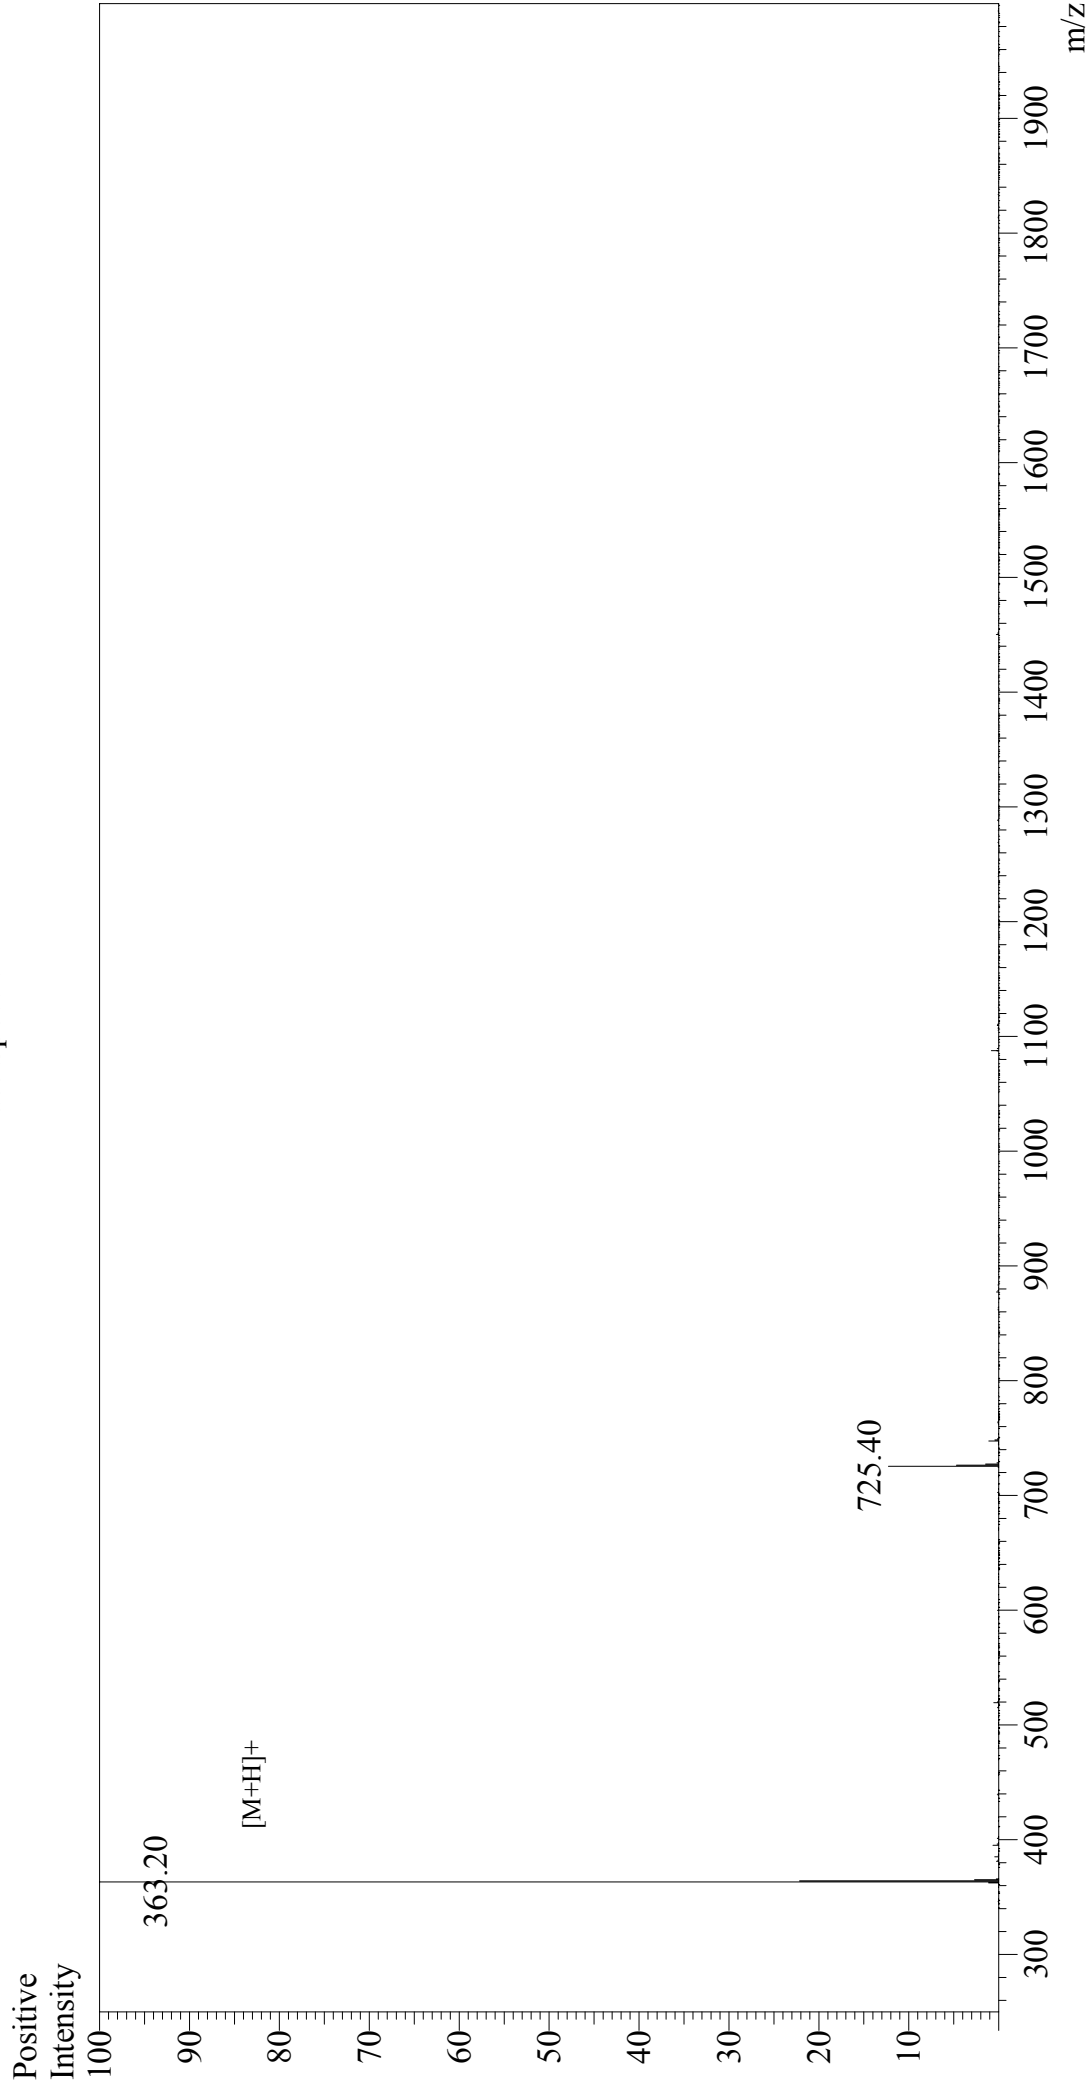

Sample Information

Acquired by :	Gary
Month-Day Processed :	05/11/18
Time Processed :	14:21:11
Injection Volume :	0.2
Sample Name :	Thyrotropin-Releasing Hormone (TRH)
Cat. No. :	RPI0112
Lot. No. :	PE2511804
Theoretical MW :	362.38
Observed MW :	362.20

Interface	:ESI
Nebulizing Gas Flow	:1.5L/min
CDL Temp	:250°C
Block Temp	:200°C

Interface Bias	
Drying Gas Flow	
T.Flow	
B.conc	

	:+4.5 kV
	:5 L/min
	:0.2 ml/min
	:50%H2O/50%MeOH