


Mass Spectrum

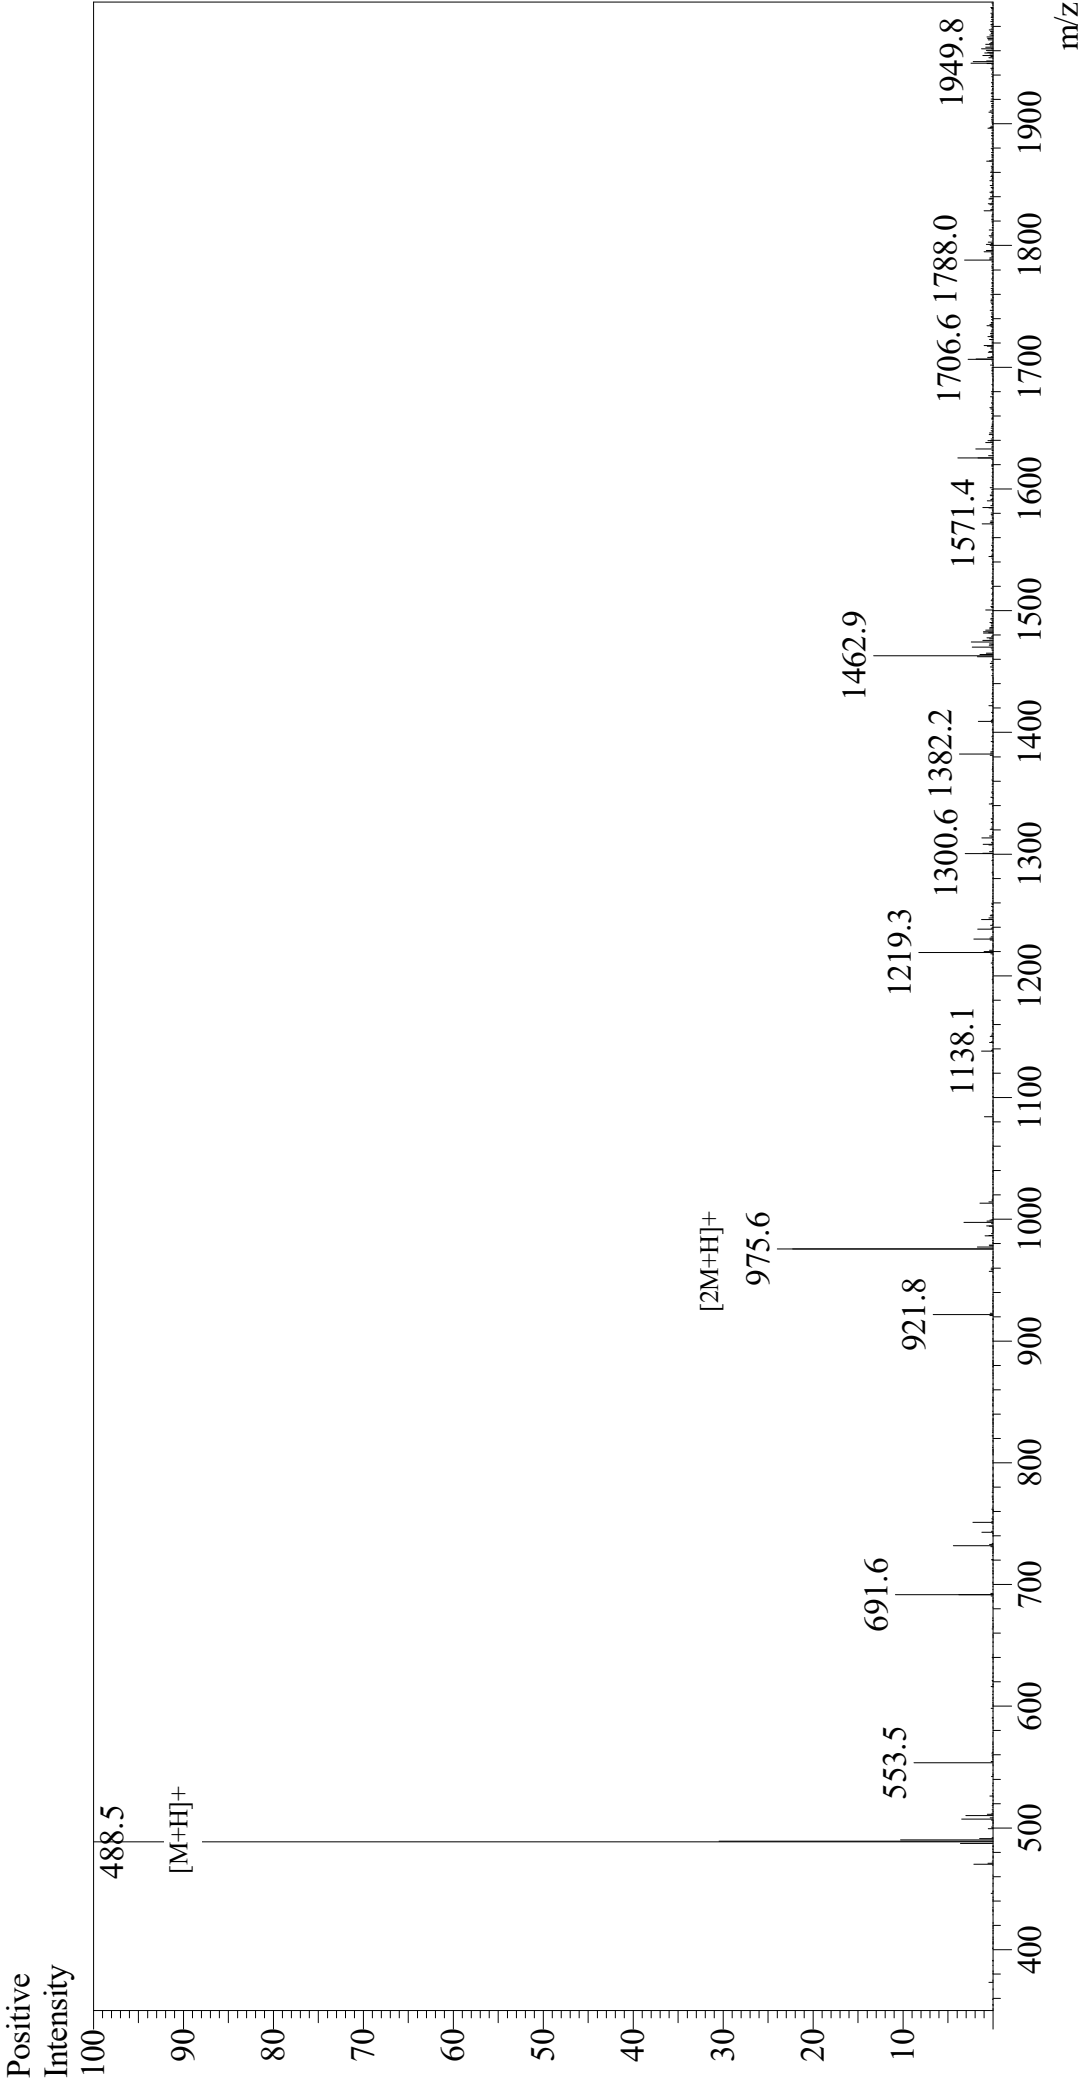

Sample Information	Equipment	: GK11010007
Month-Day Processed :	Interface	: ESI
Time Processed :	Nebulizing Gas Flow	: 1.5L/min
Injection Volume :	CDL Temp	: 250
Sample Name :	Block Temp	: 200
Cat. No. :	Drying Gas Flow	: 0.2 ml/min
Lot. No. :	T.Flow	: 50%H ₂ O/50%MeOH
Theoretical MW :	B.conc	
Observed MW :		