

Sample Name : Ghrelin, rat
 Cat. No. : RP10781
 Lot. No. : E3601919K
 Time Processed : 7:46:53
 Month-Day-Year Processed : 11/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

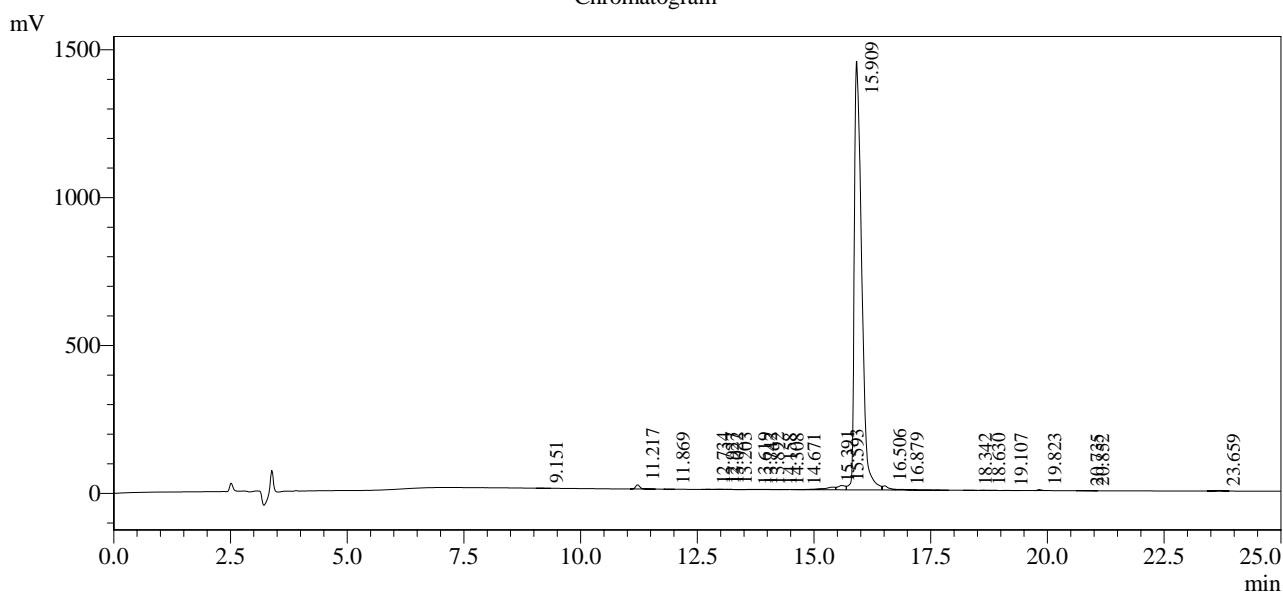

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.151	1684	207	0.010
2	11.217	95674	14112	0.574
3	11.869	1066	196	0.006
4	12.734	4463	742	0.027
5	12.927	3836	634	0.023
6	13.022	2872	620	0.017
7	13.203	3957	751	0.024
8	13.619	8594	772	0.052
9	13.742	4692	652	0.028
10	13.892	8965	632	0.054
11	14.158	2601	388	0.016
12	14.308	1328	211	0.008
13	14.671	4457	537	0.027
14	15.391	169203	8929	1.015
15	15.593	165601	14609	0.994
16	15.909	15963744	1449387	95.796
17	16.506	130829	13943	0.785
18	16.879	43030	2319	0.258
19	18.342	5420	632	0.033
20	18.630	4146	434	0.025
21	19.107	3244	330	0.019
22	19.823	19310	3282	0.116
23	20.735	2276	271	0.014
24	20.852	1906	267	0.011

Peak#	Ret. Time	Area	Height	Area %
25	23.659	11407	1184	0.068
Total		16664304	1516040	100.000