

Sample Name : β -Amyloid (1-20)
 Cat. No. : RP20162
 Lot. No. : E4837619I
 Time Processed :12:38:34
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010009

Chromatogram

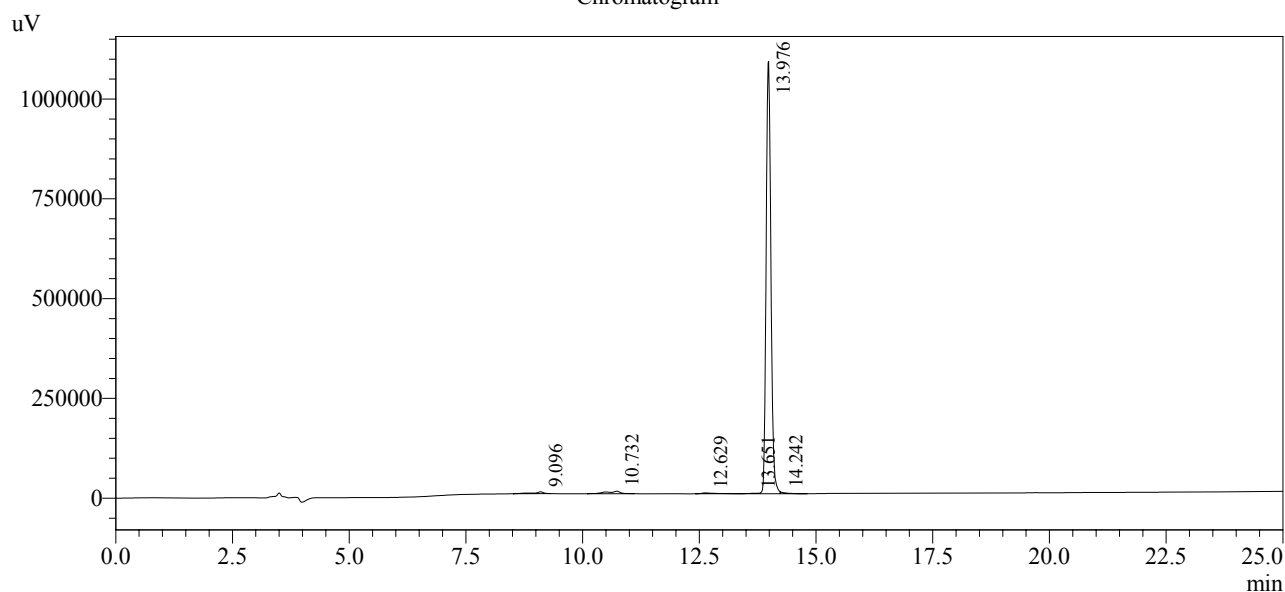

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.096	67800	4648	0.846
2	10.732	128596	6364	1.604
3	12.629	39097	2249	0.488
4	13.651	18573	1359	0.232
5	13.976	7730153	1083638	96.428
6	14.242	32320	4300	0.403
Total		8016540	1102558	100.000