

Sample Name : Ghrelin, human

Cat. No. : RP 13422 Lot. No. : PE3611807

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow: 1 ml/min
Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
35.00	Pumps	Pump A B.Conc	95	
40.00	Pumps	Pump A B.Conc	95	
45.00	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

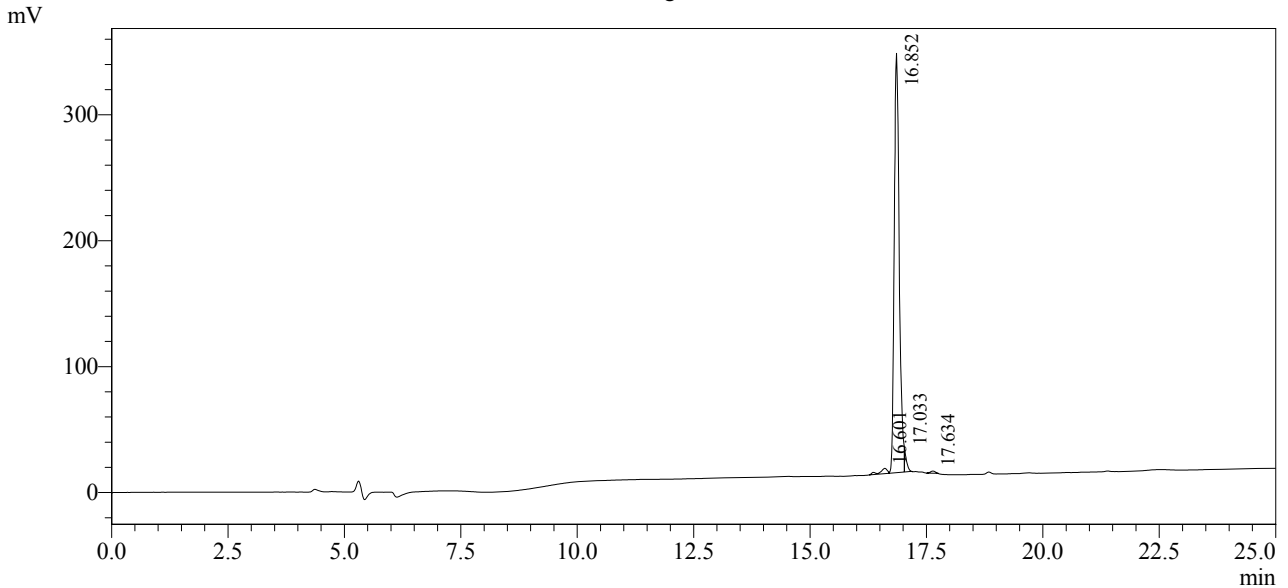

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.601	47146	4208	1.798
2	16.852	2510118	333028	95.739
3	17.033	52786	17524	2.013
4	17.634	11795	1643	0.450
Total		2621845	356403	100.000