

Sample Name : Myelin Basic Protein (MBP) (synthetic)  
 Cat No.: RP10314  
 Lot No.: E0970720D  
 Time Processed : 16:37:20  
 Month-Day-Year Processed : 05/06/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

### <Chromatogram>

mV

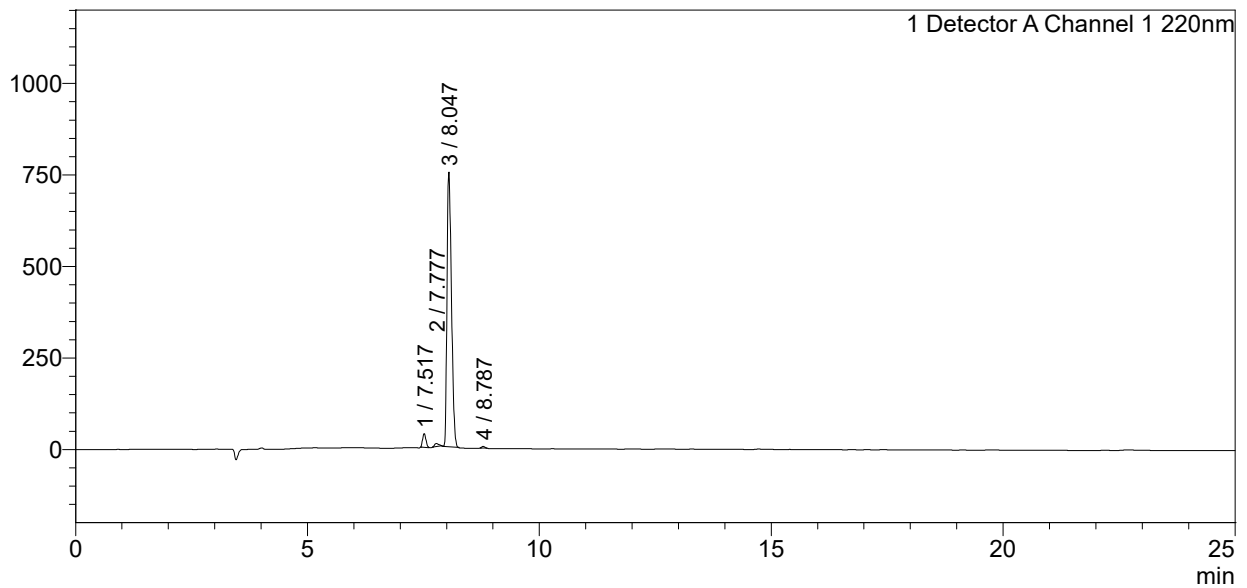

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.517	187694	37878	3.530
2	7.777	56186	8857	1.057
3	8.047	5054090	750753	95.045
4	8.787	19631	4611	0.369
Total		5317600	802098	100.000