

Sample Name : CLIP(86-100)  
 Cat. No. : RP20279  
 Lot. No. : PE17911811  
 Time Processed :4:55:32  
 Month-Day-Year Processed :11/08/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

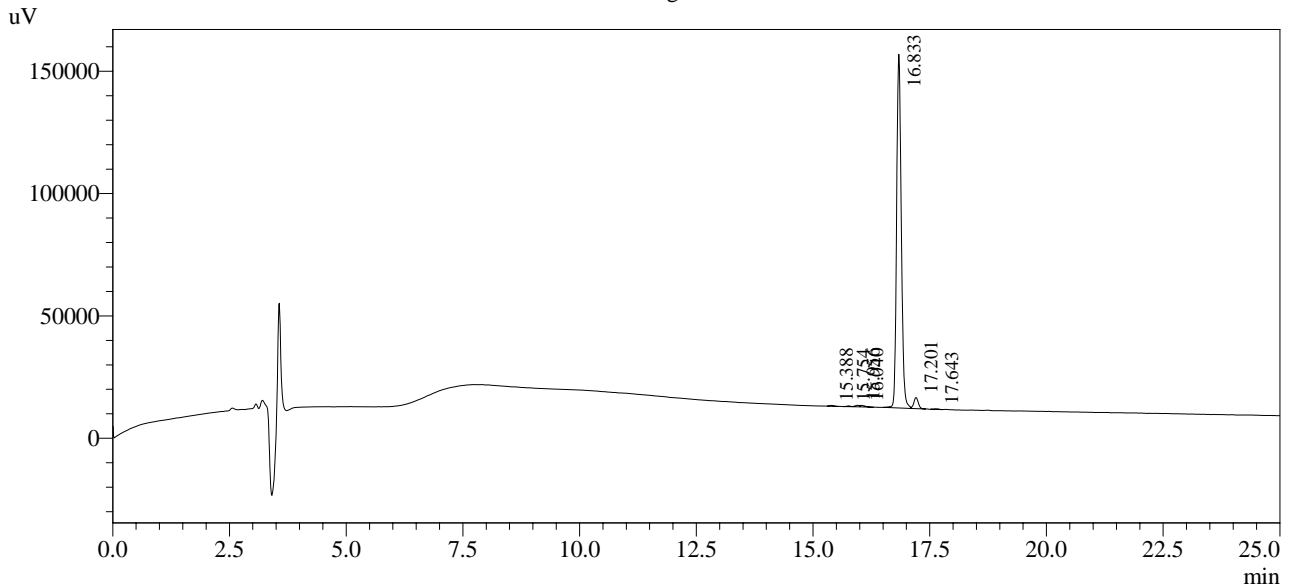

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.388	2325	323	0.222
2	15.754	1764	287	0.168
3	15.956	4449	639	0.424
4	16.040	4506	609	0.430
5	16.833	1004164	144582	95.748
6	17.201	29943	4529	2.855
7	17.643	1600	241	0.153
Total		1048752	151210	100.000