


Mass Spectrum

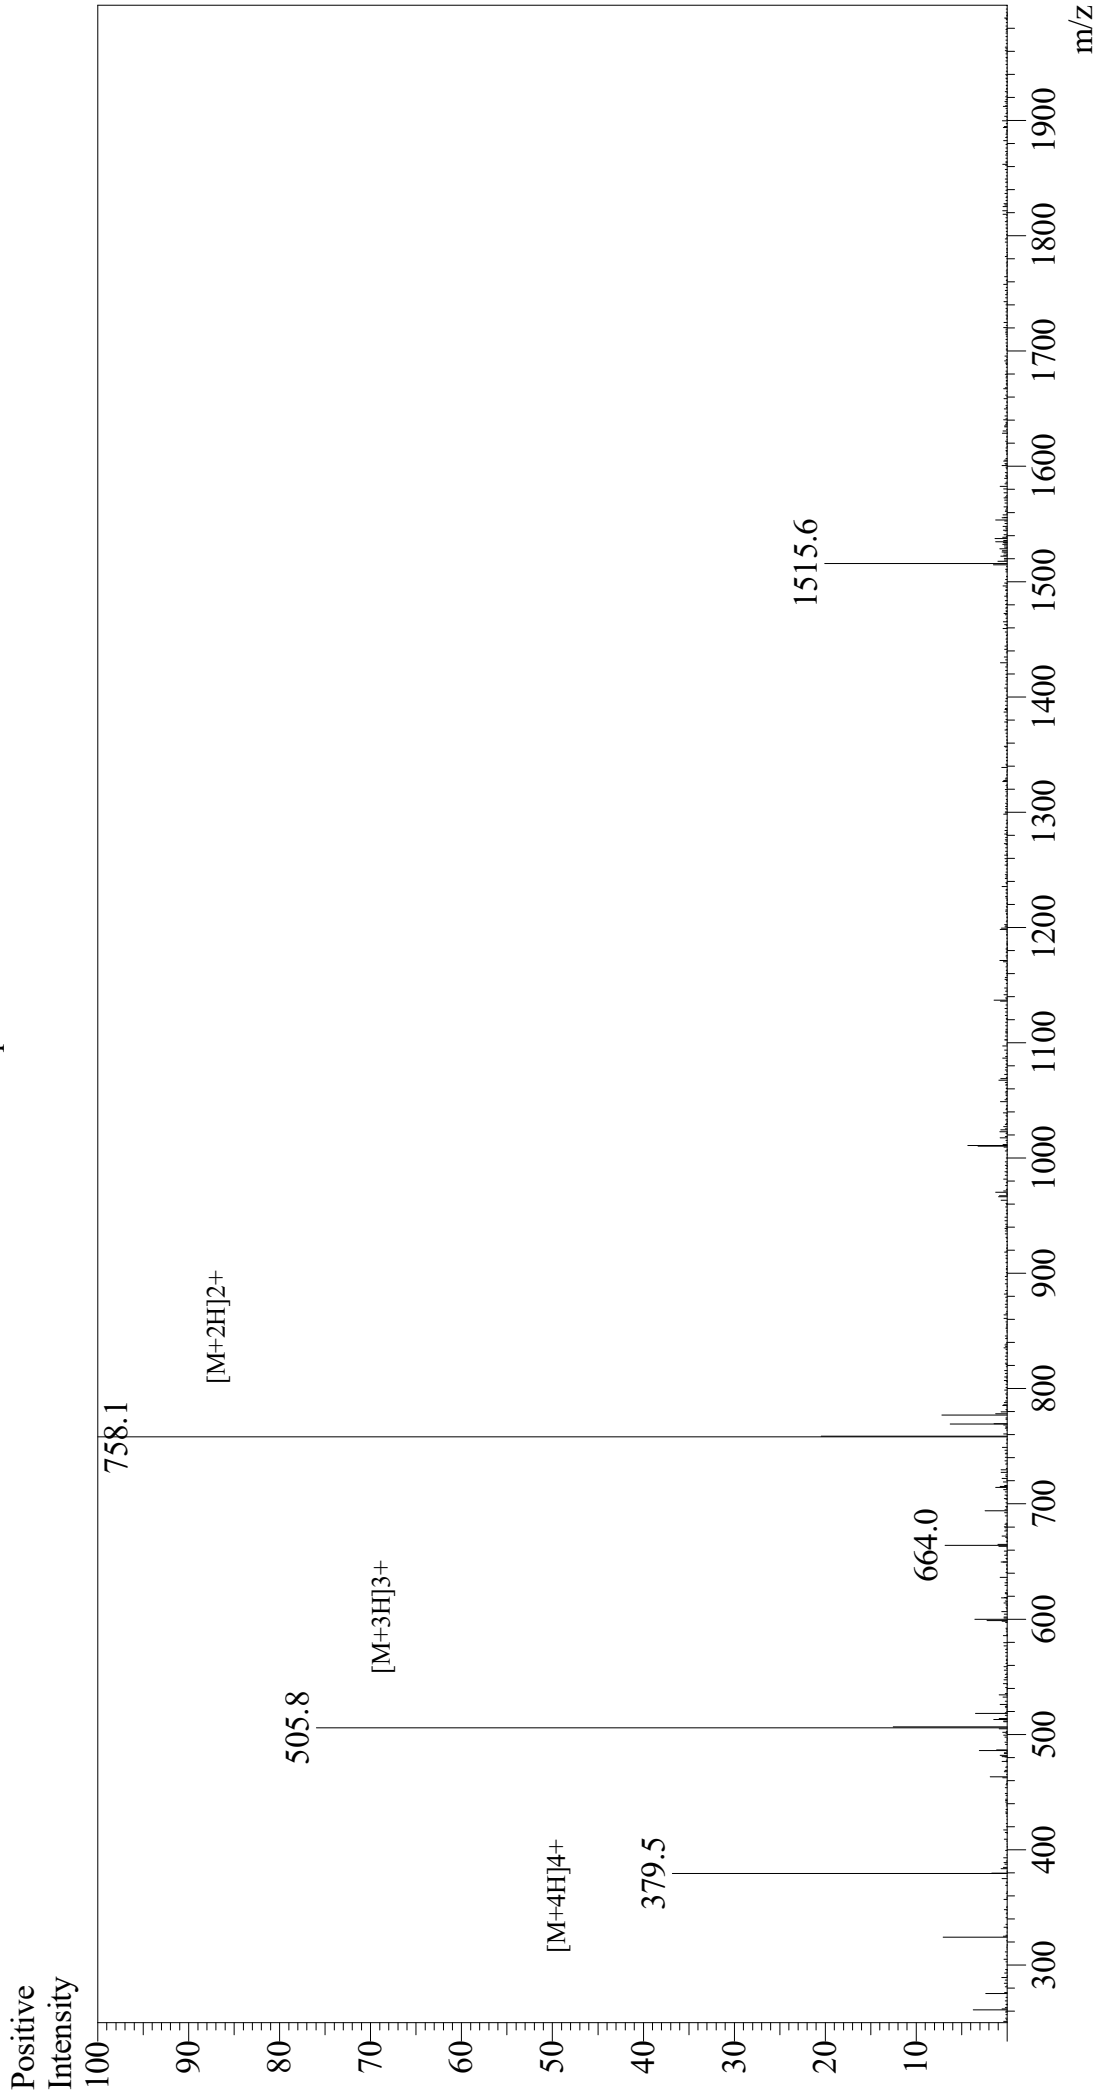

Sample Information

Month-Day Processed : 01/29/21
Time Processed : 7:05:21 AM
Injection Volume : 0.3
Sample Name : Axltide
Cat No. : RP20363
Lot No. : E0690921A
Theoretical MW : 1514.78
Observed MW : 1514.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH