

Sample Name : Bim BH3, Peptide IV
 Cat. No. : RP20339
 Lot. No. : E5706519F
 Time Processed : 10:21:38
 Month-Day-Year Processed : 06/30/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

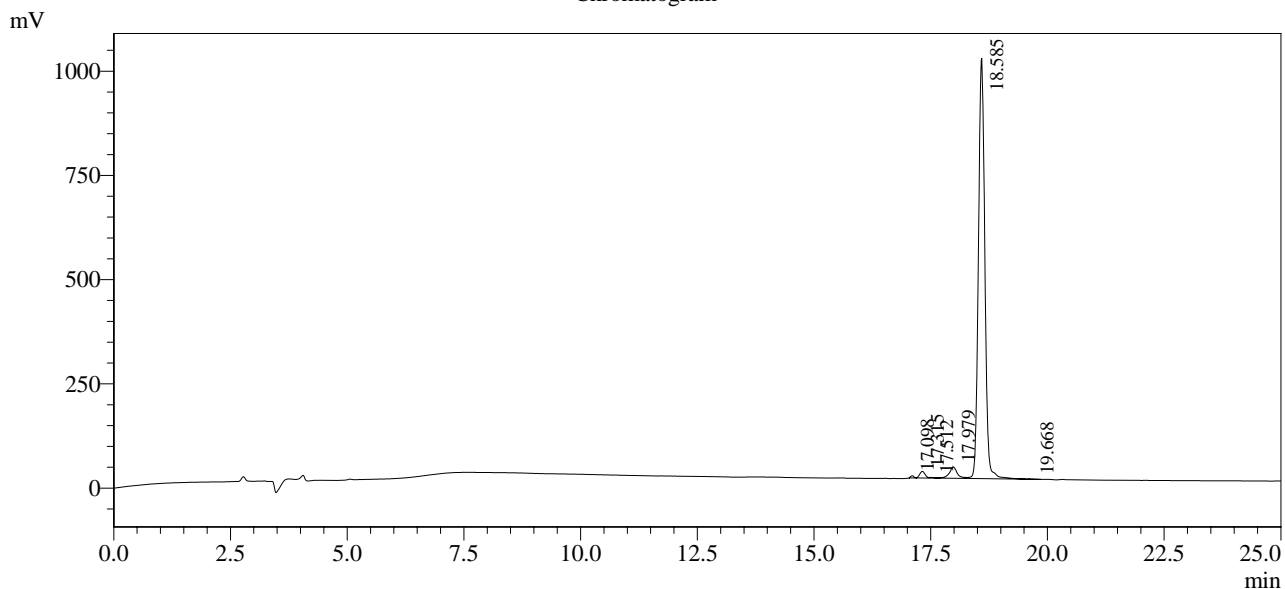

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.098	24727	5268	0.244
2	17.315	128408	15906	1.268
3	17.512	9785	1597	0.097
4	17.979	323833	27326	3.197
5	18.585	9640456	1008257	95.175
6	19.668	1975	268	0.019
Total		10129184	1058622	100.000