

Sample Name :TAT
 Cat. No. : RP12784
 Lot. No. : E2278020A
 Time Processed :7:41:04
 Month-Day-Year Processed :01/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

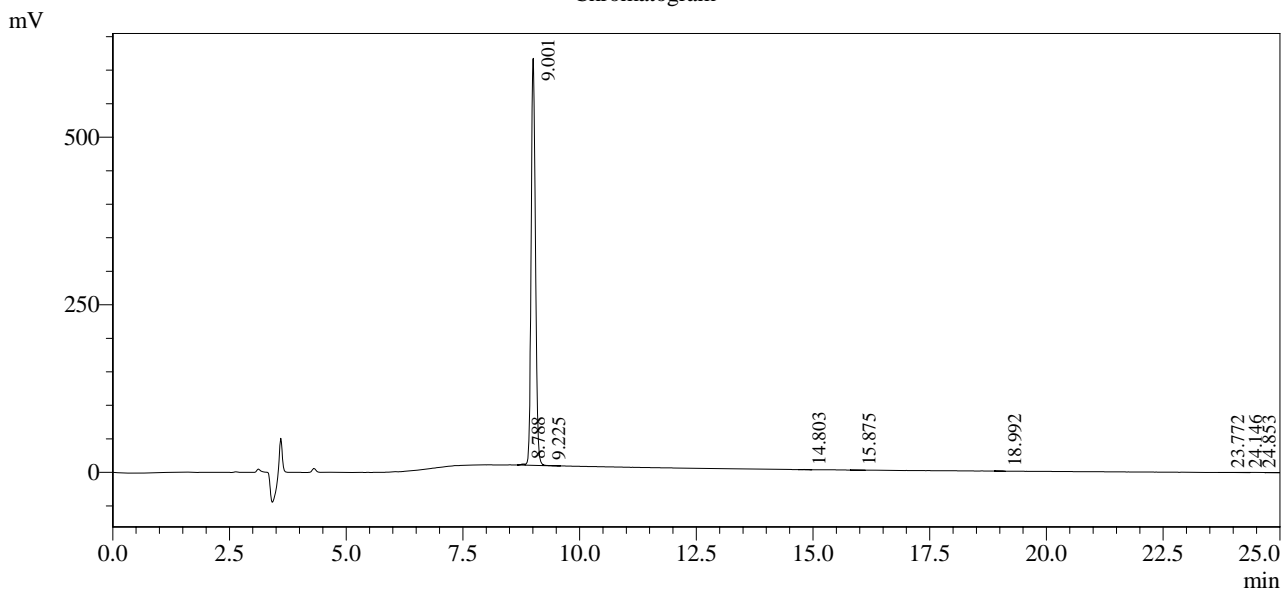

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.788	9834	1734	0.251
2	9.001	3897681	607304	99.344
3	9.225	4240	1165	0.108
4	14.803	1269	211	0.032
5	15.875	1180	125	0.030
6	18.992	1439	235	0.037
7	23.772	1558	170	0.040
8	24.146	2331	296	0.059
9	24.853	3873	416	0.099
Total		3923406	611655	100.000