


# Mass Spectrum

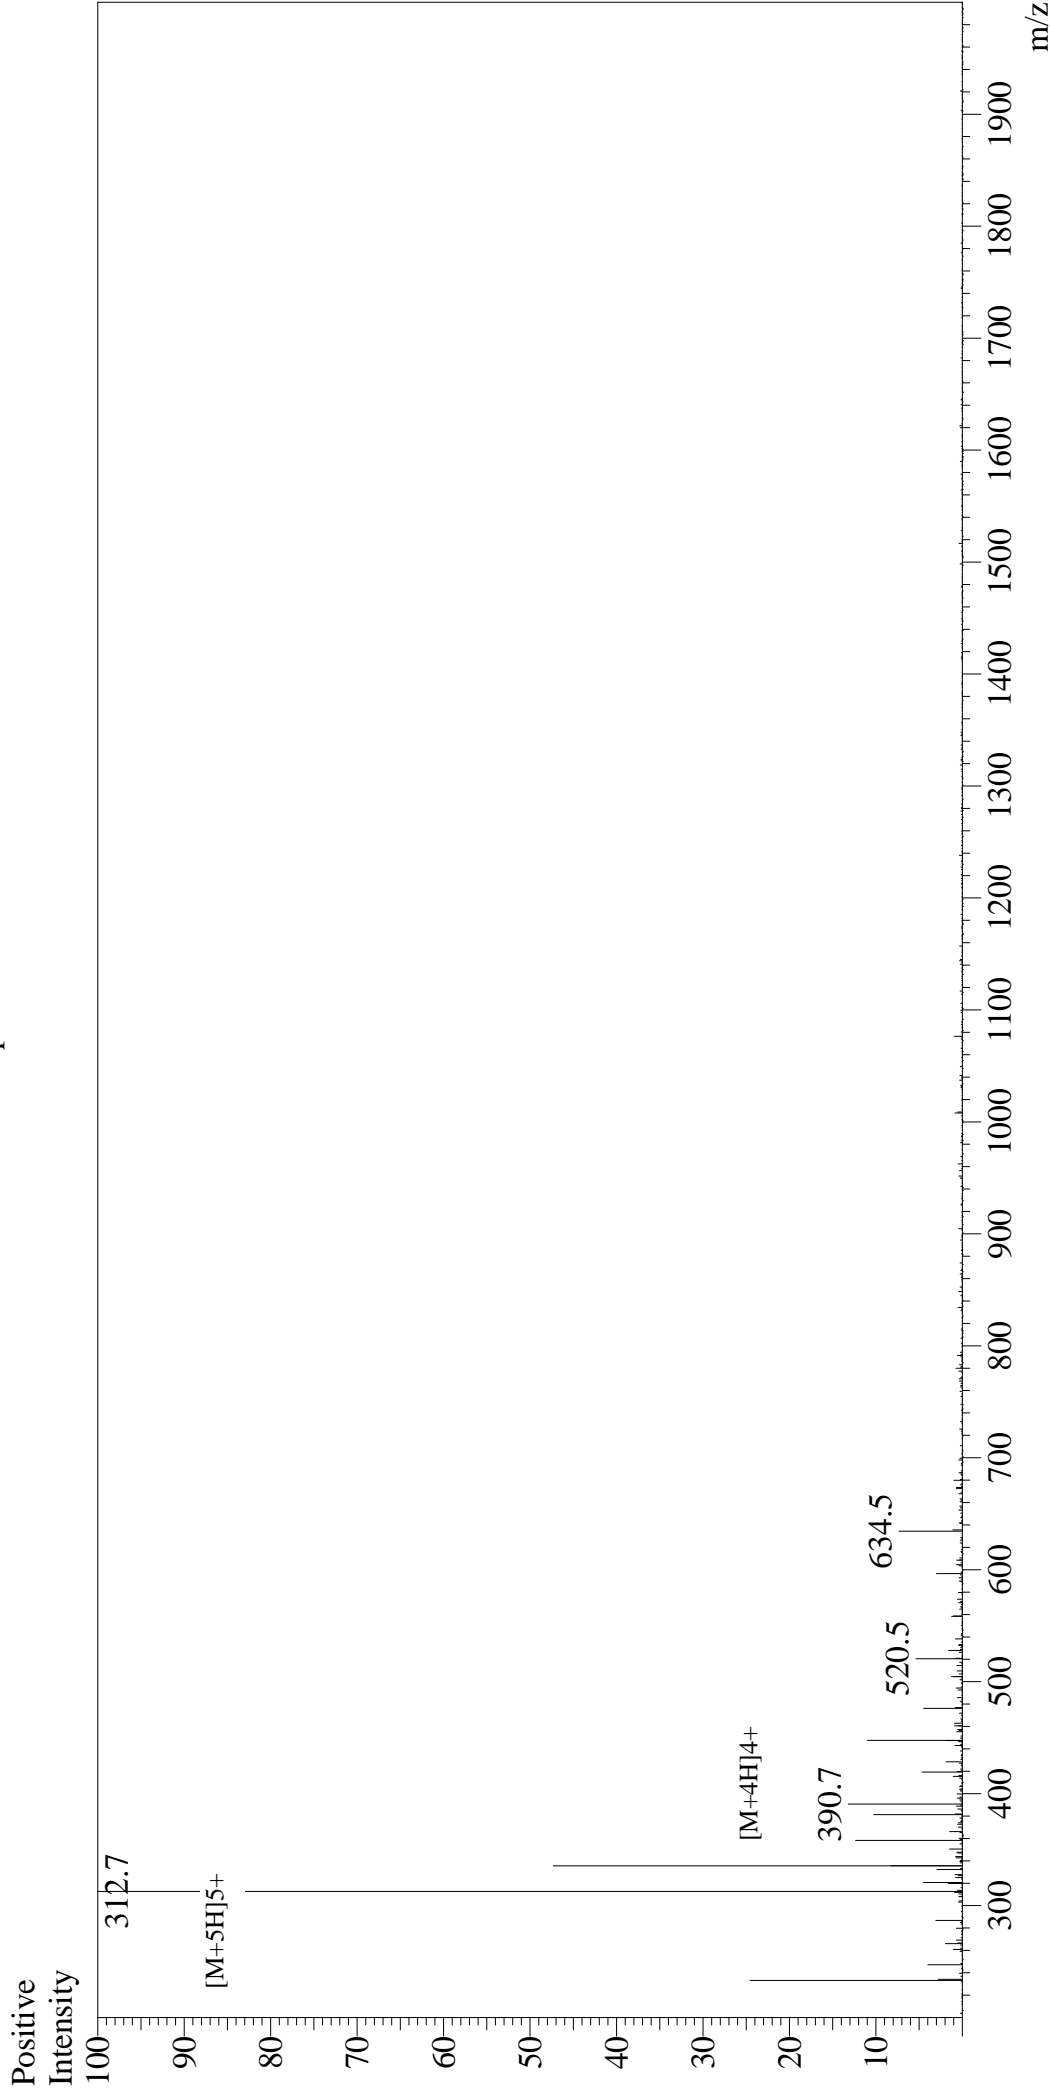

## Sample Information

User : Gary  
Month-Day Processed : 01/13/20  
Time Processed : 22:44:48  
Injection Volume : 0.3  
Sample Name : TAT  
Cat No. : RP12784  
Lot No. : E2278020A  
Theoretical MW : 1558.85  
Observed MW : 1558.5

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200  
Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH